
skeletal dynamics®
UNDERSTANDING THE UPPER EXTREMITY

SURGICAL TECHNIQUE GUIDE

GEMINUS®
distal radius system

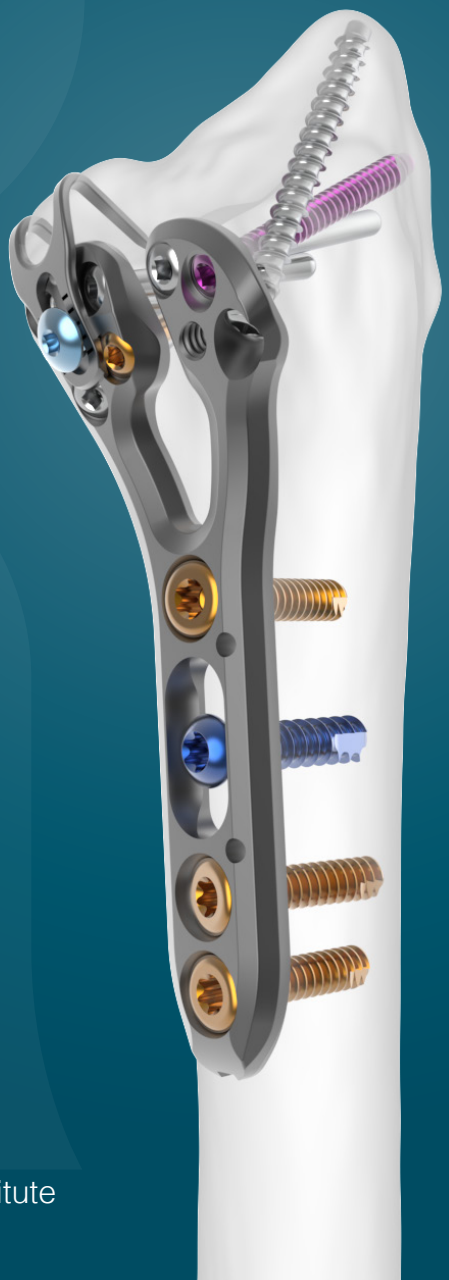

As described by:
Jorge L. Orbay, M.D.
Miami Hand & Upper Extremity Institute



TABLE OF CONTENTS


1. Extended FCR Surgical Approach....4
2. Polyaxial Locking Screw Surgical Steps....20
3. Optional Hook Plate Extension Surgical Steps....24
4. Geminus XL® Surgical Steps....29
5. Distal Fragment First Surgical Technique....34
6. Optional Drill Block Usage....38
7. PROTEAN Fragment Plate Surgical Steps....42
8. Dorsal Spanning Plate Surgical Steps....52
9. Optional Plate Bending Technique....59
10. Instrumentation Tray Set Configuration....60
11. GEMINUS® Volar Plate Specifications....61
12. PROTEAN® Fragment Plate Specifications....61
13. Single Use Instruments....62
14. Screw Caddy Set Configuration....63
15. PLS and HPE Module Set Configuration....65
16. GEMINUS XL® Module Configuration....67
17. Dorsal Spanning Plate Set Configuration....67
18. Dorsal Spanning Plate Specifications....67
19. Optional Drill Block Module....68

01 EXPOSURE

Assess the fracture radiographically to determine the plate length needed.


Start the incision distally at the level of the trapezial ridge (★), then cross the wrist flexion creases in a zig zag fashion. Extend the incision over the course of the Flexor Carpi Radialis (FCR) tendon to the proximal most fracture line.

Note: GEMINUS Volar Plate size options are detailed in the specifications located on page 61 of this surgical technique guide.

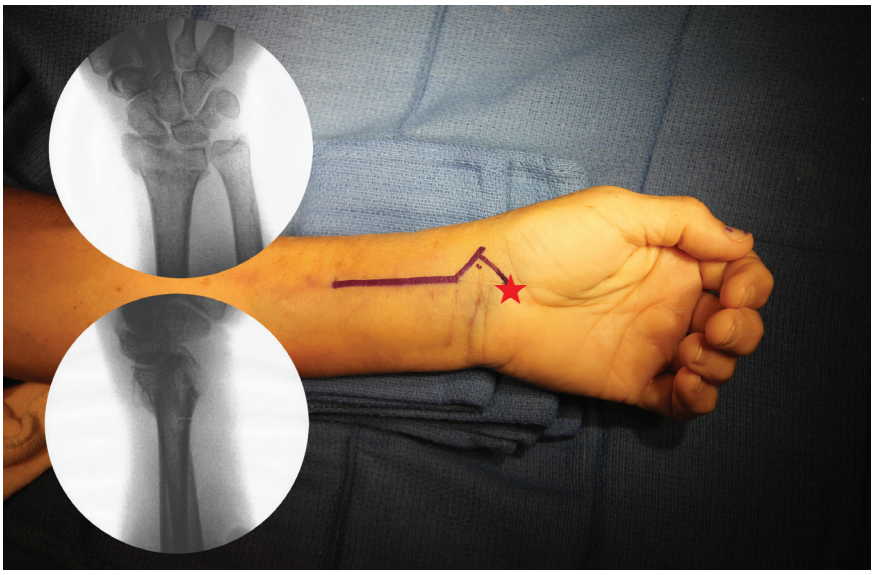

02 RELEASE THE FCR TENDON SHEATH


Open the sheath of the FCR tendon and dissect distally past the level of the superficial radial artery.

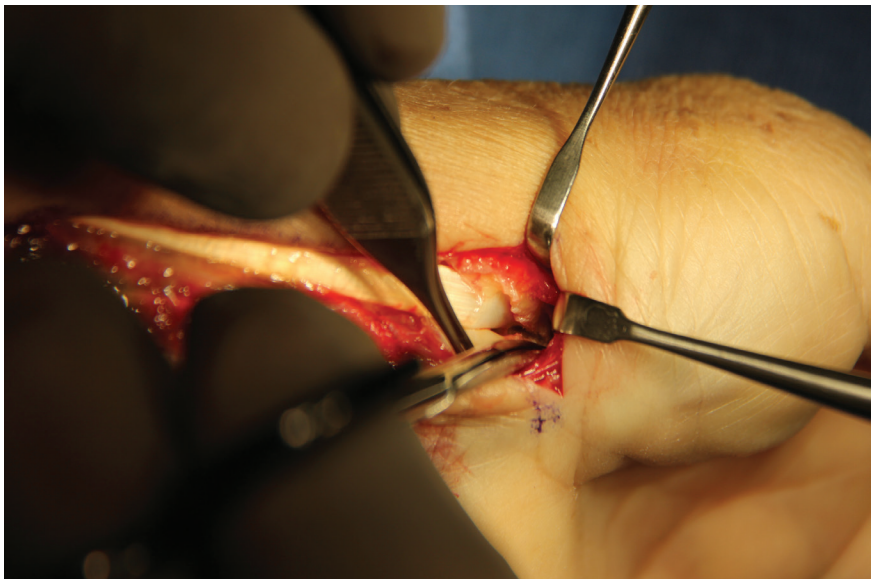

03 CROSSING THE DEEP FASCIA


Retract the FCR tendon ulnarly while protecting the median nerve.

Incise through the floor of the FCR tendon sheath distally to the level of the trapezium.

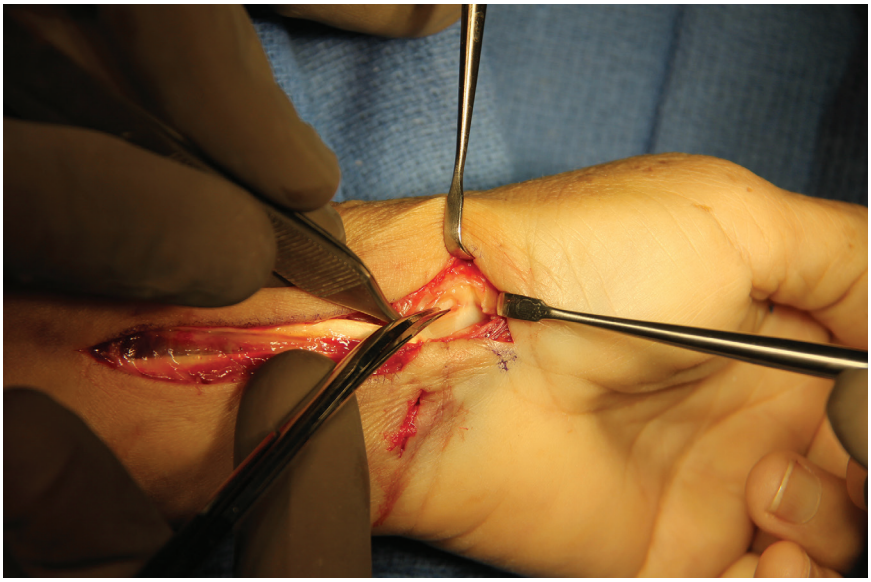

04 MID-LEVEL DISSECTION

Widely develop the subtendinous space of Parona and expose the Pronator Quadratus (PQ) muscle.

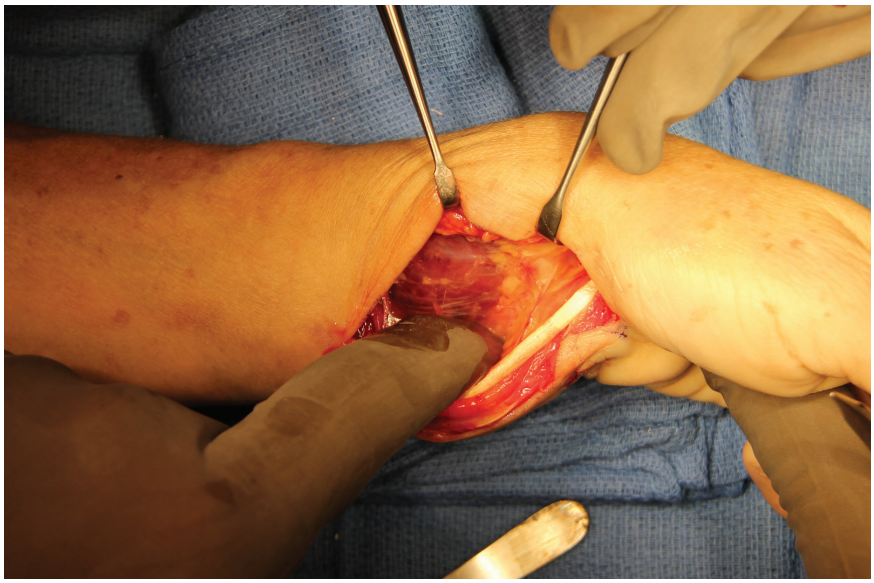



05 IDENTIFYING THE WATERSHED LINE

Identify and mark the location of the watershed line; it is best found by palpating for the volar rim of the lunate fossa (★).

Note: The Transitional Fibrous Zone (TFZ) is a 1cm wide band of fibrous tissue located between the watershed line and the PQ muscle.


The TFZ must be elevated to properly expose the radius and position the plate.

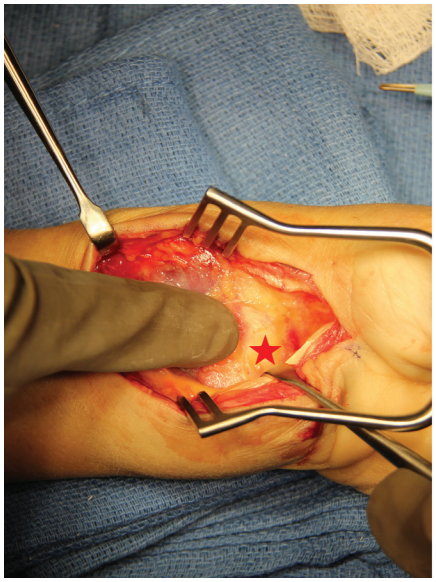

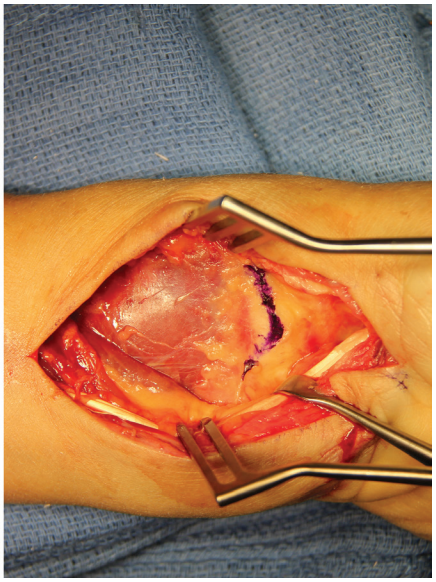

06 THE RADIAL SEPTUM


The radial septum is a complex fascial structure formed by the intermuscular membrane, the first extensor compartment, the insertion of the brachioradialis and the distal part of the FCR tendon sheath.

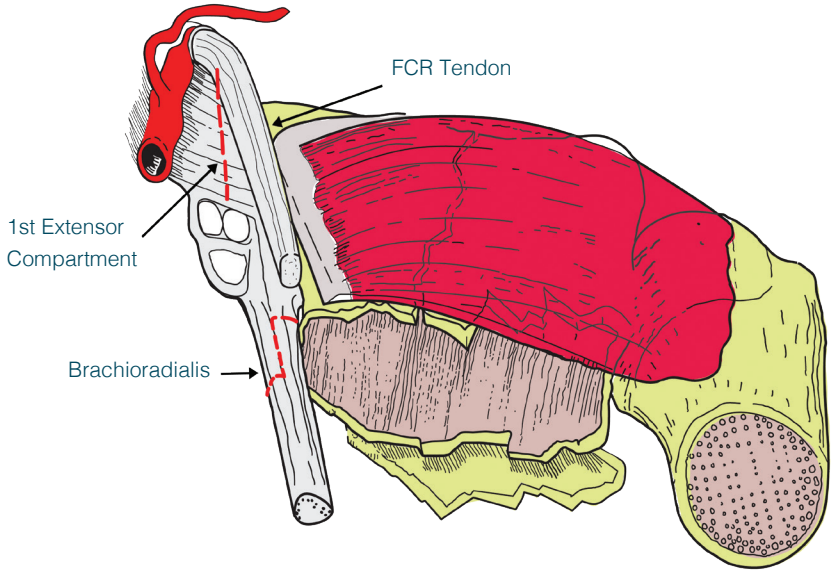


07 RELEASING THE RADIAL SEPTUM

Release the radial septum by incising the intermuscular membrane at the radial border of the brachioradialis.

Carry this release distally while protecting the radial artery and sensory nerve.

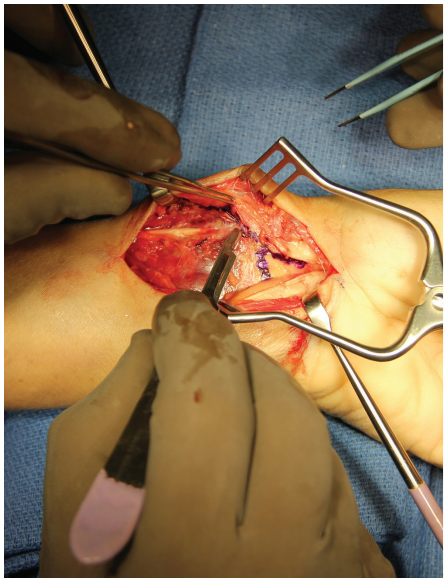

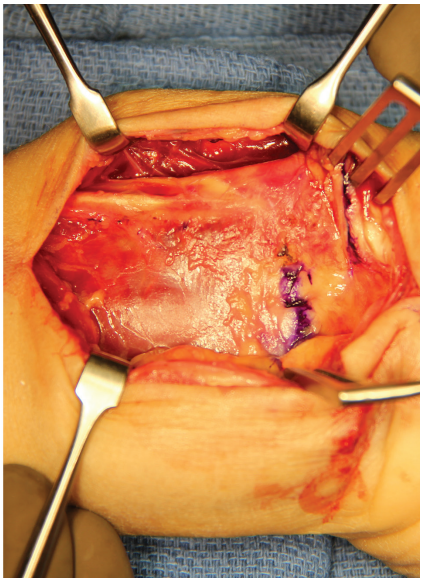



08 ELEVATING THE PQ MUSCLE

Incise and elevate the TFZ using a scalpel to properly expose the radius and position the plate.

The PQ muscle is frequently avulsed from its distal attachment to the TFZ. Use a periosteal elevator to lift the PQ muscle from the radius.

Note: The origin of the Flexor Pollicis Longus (FPL) muscle may be partially released for added exposure.

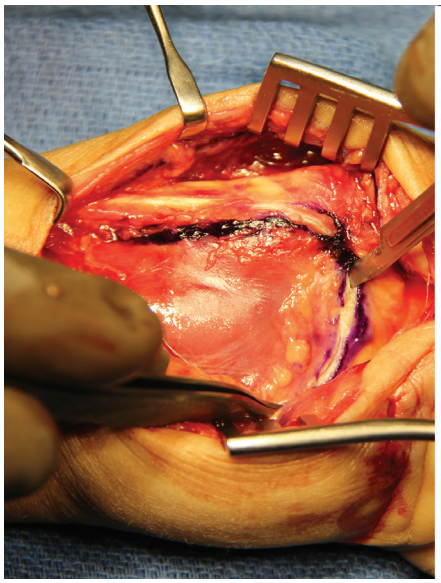


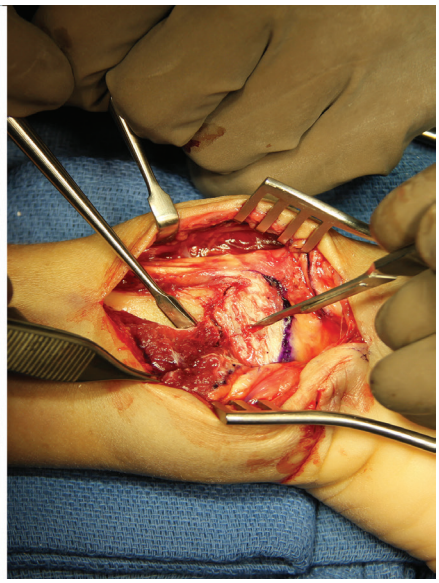


09 RELEASE OF THE BRACHIORADIALIS

Release the insertion of the brachioradialis using a step cut tenotomy in order to facilitate later repair.

Note: The brachioradialis is the prime deforming force of the distal radius fracture.

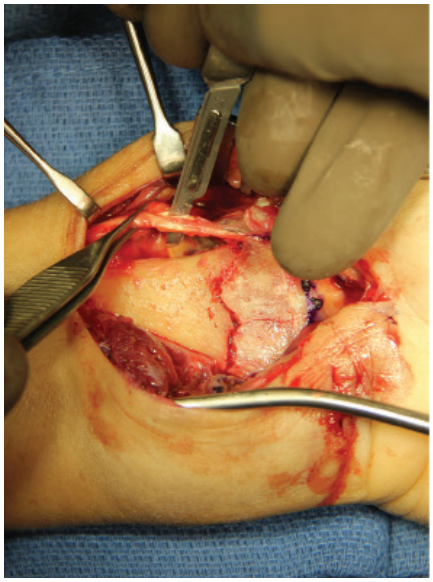


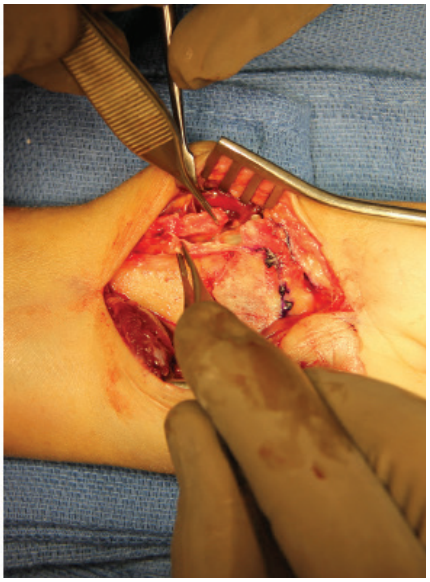


10 INTRA-FOCAL EXPOSURE

Using bone-holding forceps, rotate the proximal fragment into pronation.

Note: This provides ample exposure of the fracture, allowing for a thorough debridement and access to articular fragments.

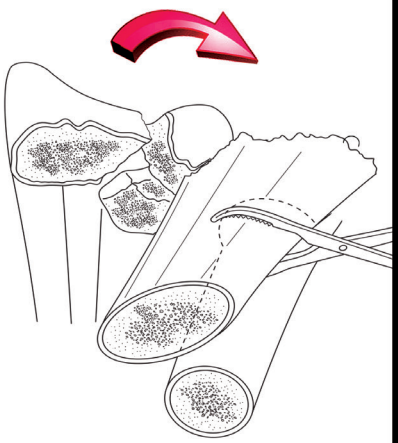

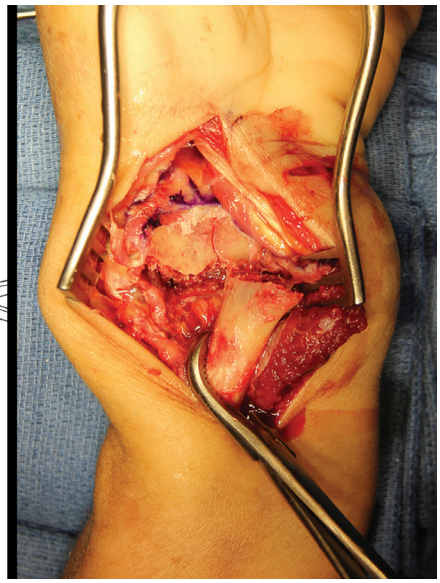




Forceps, Bone Holding

11 DEBRIDING THE FRACTURE SITE


It is necessary to remove the clot, fibrous tissue and callus to achieve a proper reduction for complex articular or partially healed fractures.

Note: Preserve the soft tissue attachments to the medial aspect of the proximal fragment. Here, perforators from the anterior interosseous artery feed the proximal radial shaft.

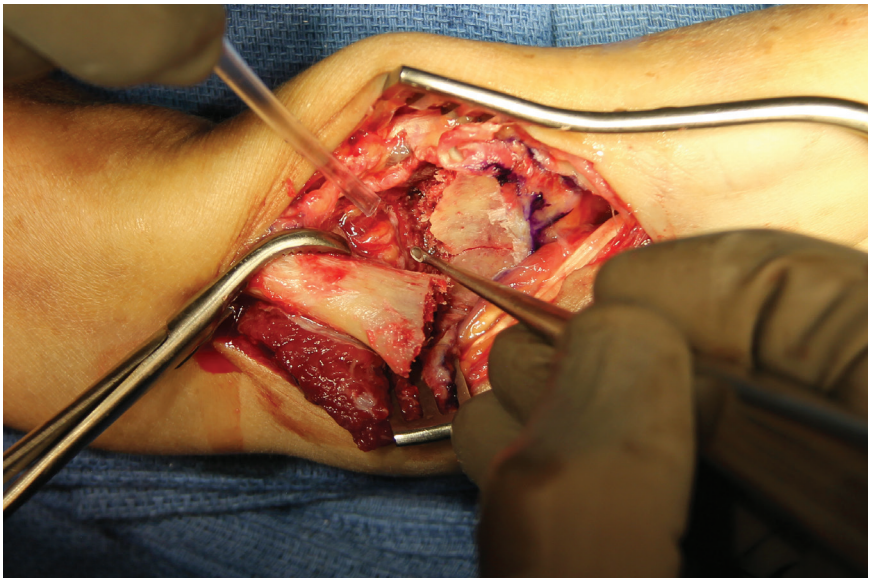

12 RELEASING THE DORSAL PERIOSTEUM

In some inveterate fractures, it may be necessary to release or excise the thickened dorsal periosteum to achieve a proper reduction.

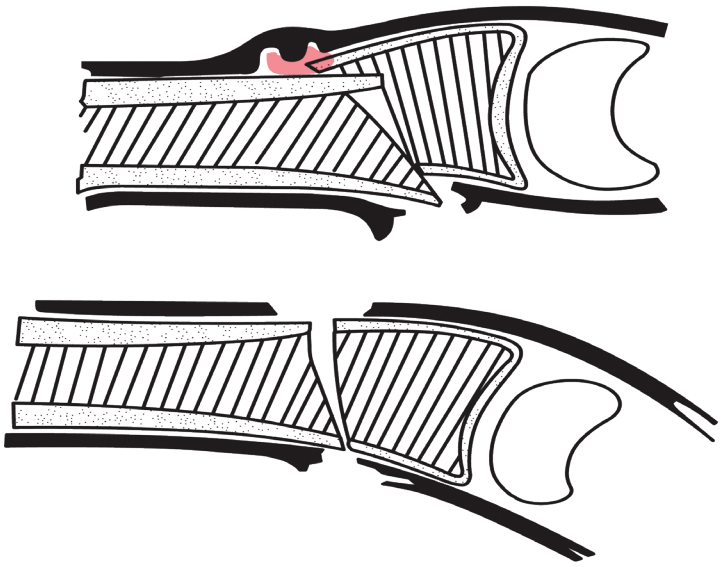


13 INITIAL FRACTURE REDUCTION

Supinate the proximal radius back into place and reduce the volar cortex.

To facilitate reduction, provide traction to the hand and use a bolster.

Note: For fractures which require an XL plate, refer to the GEMINUS XL surgical steps located on pages 29-33 of this Surgical Technique Guide.

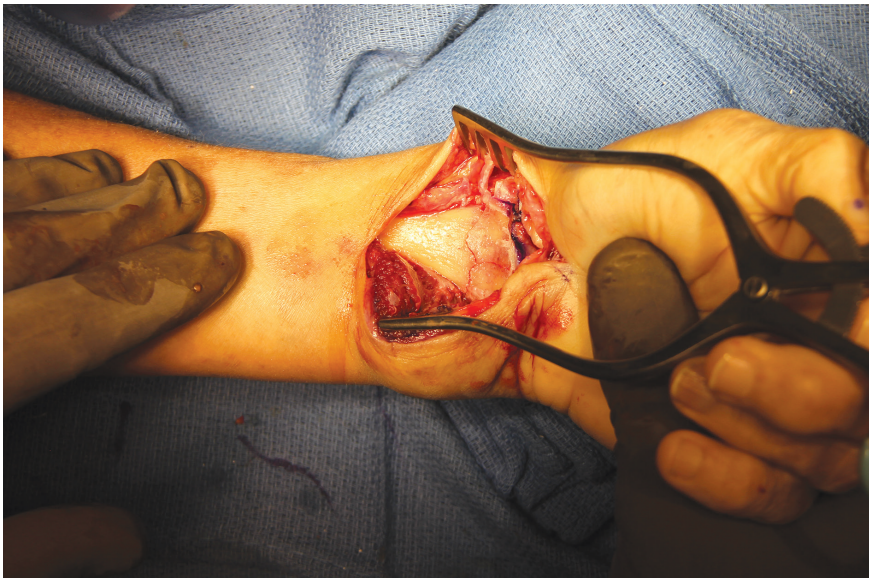


14 PRE-LOADING K-WIRE A.I.M.ING GUIDES

Select two A.I.M.ing Guides and thread them into the pre-loaded drill guide (PDG) at the proximal ulnar hole (A) of the lunate head, and at the most radial hole (B) of the scaphoid head.

Note: Each A.I.M.ing Guide positions the K-wire in the axis of the corresponding peg.

The Square Tip Driver is designed to break in an area that will allow for easy removal if excess torque is applied.

For the Distal Fragment First technique, refer to page 28.

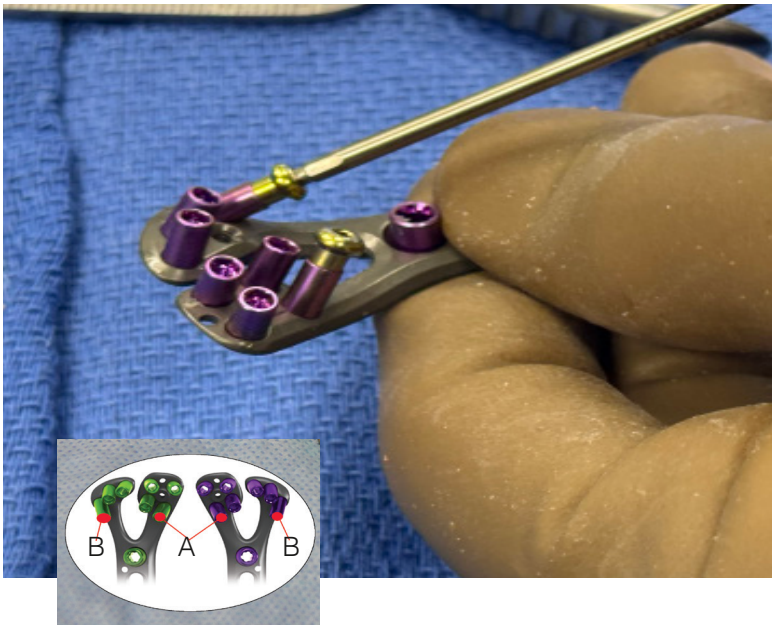



Driver, Square Tip 2.0mm


15 PROXIMAL PLATE FIXATION

Position the lunate head of the GEMINUS Plate approximately 2mm proximal to the volar rim of the lunate fossa (watershed line).

Align the proximal portion of the plate to the radial shaft, then drill through the center of the gliding hole using the 2.5mm bit.

Using the appropriate scale of the Depth Gauge, measure and then insert a 3.5mm compression screw (Non Locking Cortical Screw).

Note: To avoid contact with flexor tendons, the plate must be applied just proximal to and below the watershed line.

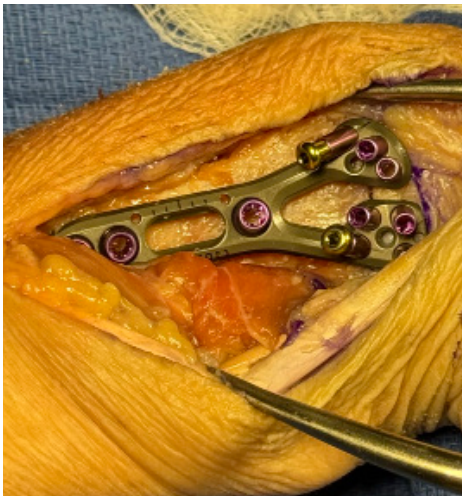





Drill, 2.5mm



Driver, Quick Connect T10



Depth Gauge, Standard

16 FINAL FRACTURE REDUCTION

Using the GEMINUS plate as a template, apply longitudinal traction and direct pressure over the dorsal aspect of the radius to reduce the fracture.

It is important that the distal edge of the plate is flush to the surface of the radius.




17 LUNATE FOSSA - PROVISIONAL FIXATION

Reduce and fix the lunate fossa fragment(s) to the lunate head of the GEMINUS plate using a 1.6mm K-wire through the A.I.M.ing Guide.

Confirm the proper placement of the K-wire approximately 2mm below the subchondral bone in the 20˚ elevated lateral view (1) and below the subchondral plate of the DRUJ in the AP view (2). A tangential view of the distal radius is useful at this step(3).



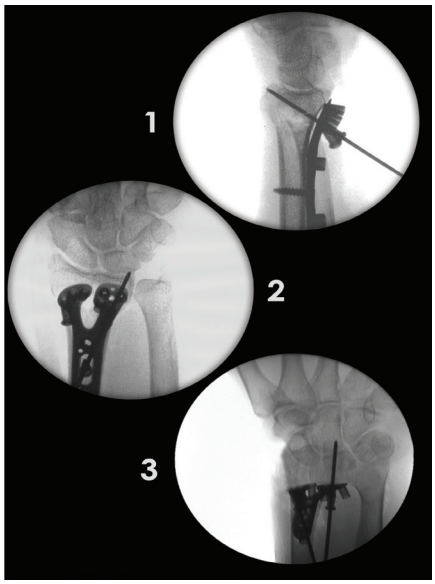




K-wire, 1.6mm


18 SCAPHOID FOSSA - PROVISIONAL FIXATION

If present, reduce and fix the scaphoid fossa fragment to the previously reduced lunate fossa fragment(s).

Once proper placement is confirmed, bend the K-wires out of the way to facilitate drill insertion.

Note: K-wires also aid in centering the plate to the distal fragments.

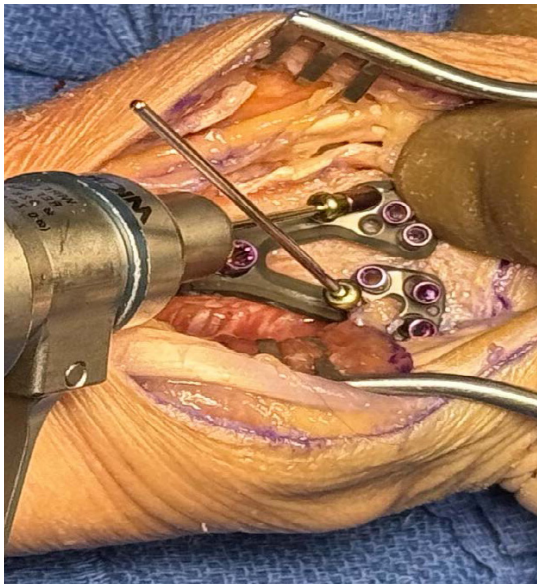

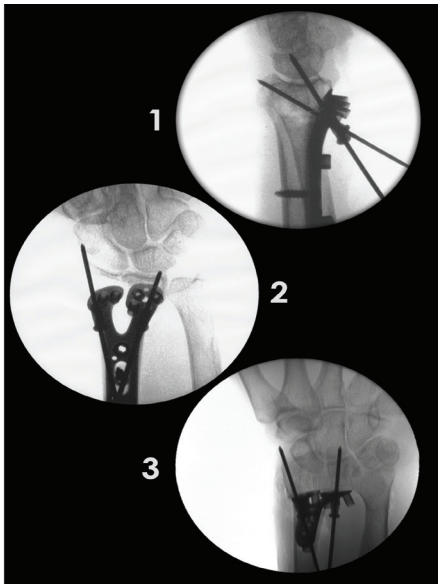


19 PILOT HOLE PREPARATION

Using the 2.0mm bit, drill through the PDG of the medial proximal hole of the lunate head (A).

Measure the peg length using the Depth Gauge taking note of the appropriate scale.

Note: Each hole should be prepared sequentially.

Caution: Prevent excessive peg length as this can potentially cause tendon irritation.

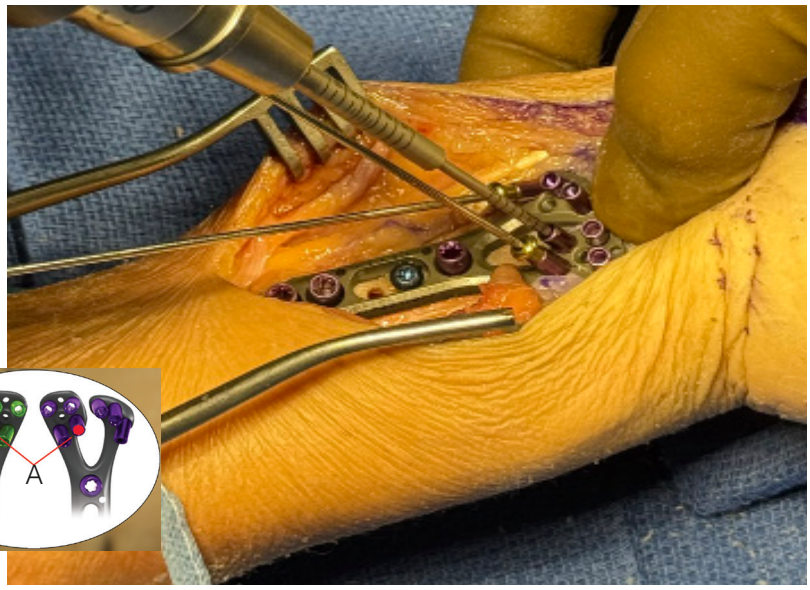



Drill, 2.0mm



The Depth Gauge has a dual scale to reflect measurements either through the pre-loaded drill guides (top scale) or without pre-loaded drill guides (bottom scale).

20 PLATE COMPRESSION


Remove the PDG using the Peg Driver.


Insert a High Compression Locking Peg to compress the plate down to the bone.

Apply direct pressure over the dorsal aspect of the radius prior to locking the screw to the plate to achieve full compression.

Note: High Compression Locking Pegs help to reduce and stabilize dorsal fragments by means of a differential pitch effect.


If re-drilling of the hole is necessary, use the appropriate Thread-in Drill Guide to facilitate this step.

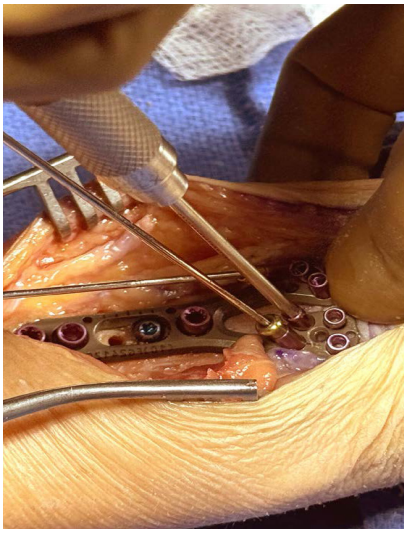

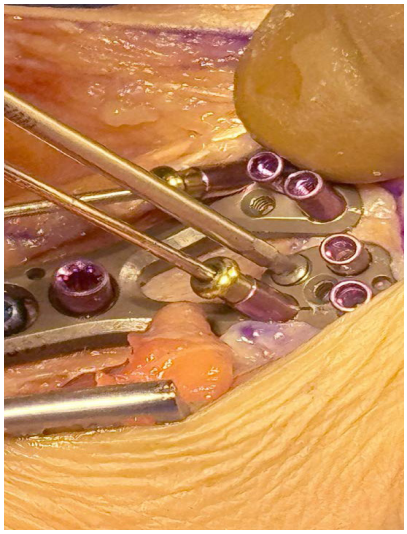



High Compression Locking Peg




Thread-In Drill Guide, 2.0mm

21 PEG PREPARATION

Prepare all remaining available peg holes and insert locking pegs or screws.

Now remove the K-wires and A.I.M.ing guides and complete the holes.

Warning: Use only one High Compression Locking Peg per bony fragment.

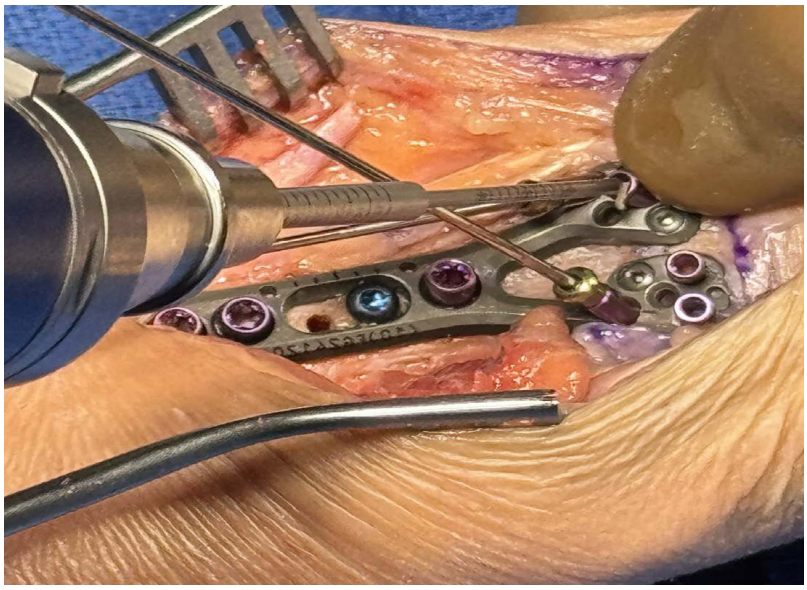



Smooth Locking Peg



Threaded Locking Peg


22 POLYAXIAL LOCKING SCREW OPTION

In situations where a peg is not optimally positioned, the Polyaxial Locking Screw (PLS) allows you to insert a screw in a desired trajectory different than the one determined by the plate.

Please refer to the “Polyaxial Locking Screw Surgical Steps” section located on page 20 of this surgical technique to review the steps and instrumentation.

Warning: Do not use a PLS in the most distal hole(s) of the lunate head.

Use only one PLS per head.

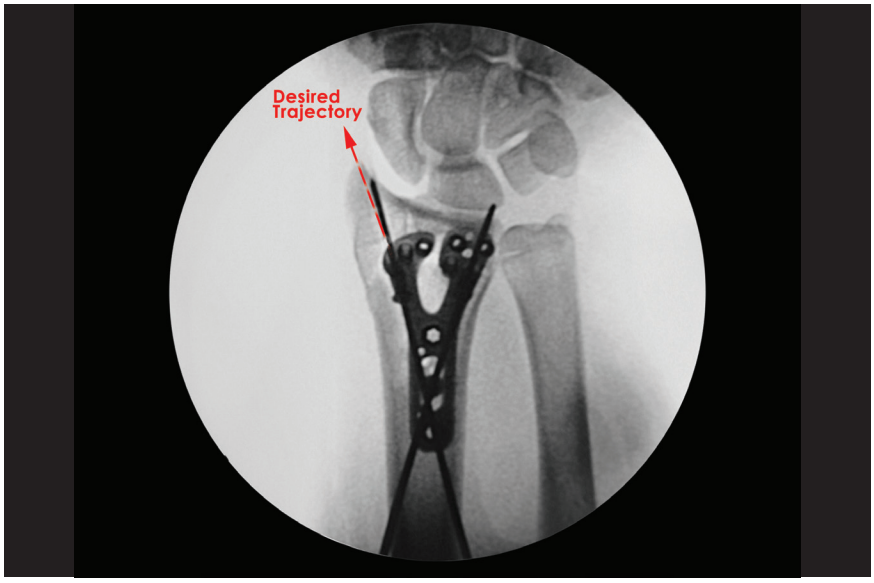




Polyaxial Locking Screws, Cannulated

23 HOOK PLATE EXTENSION OPTION

The GEMINUS Volar Plating System includes a Hook Plate Extension (HPE) to provide increased fixation of the volar marginal fragment (VMF).

After the fracture has been reduced and fixed with the GEMINUS plate, an unstable VMF may be noted.

Please refer to the "Hook Plate Extension (HPE) Surgical Steps" section located on page 24 of this surgical technique to review the steps and instrumentation.

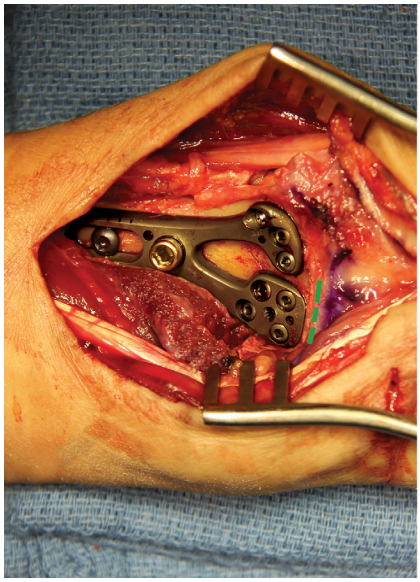



24 PROXIMAL PLATE FIXATION

Drill through the PDG's using the 2.5mm bit.


Measure the screw length using the Depth Gauge taking note of the correct scale.


Remove the PDG using the T-10 driver and insert the appropriate length 3.5mm compression screw (Non Locking Cortical screw) (1) .


If using a 3.5mm locking screw instead, you must enlarge the near cortex drill hole using the tip of the T-10 driver (2).

Now insert the appropriate length 3.5mm Cortical Locking screw (3).

Repeat for all remaining proximal screw holes.

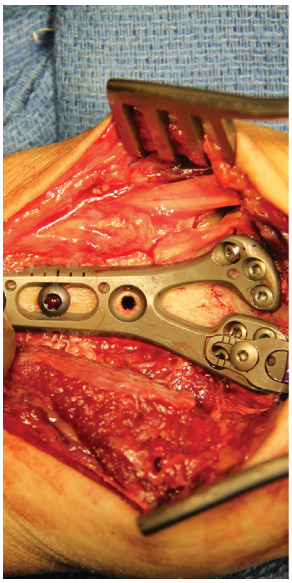

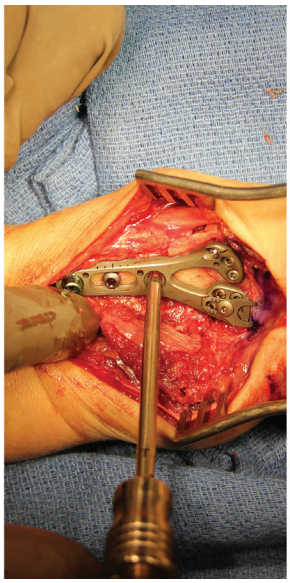

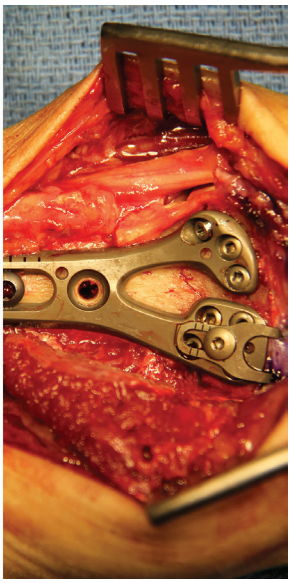



Driver, Quick Connect T10




Thread-In Drill Guide, 2.5mm

25 FINAL RADIOGRAPHS


Confirm reduction, proper peg length and placement in the AP view (1), a 20˚ elevated lateral fluoroscopic view (2) and by rotating the wrist under fluoroscopy using a tangential view (3).

Warning: Remove ALL PDG's and A.I.M.ing Guides.

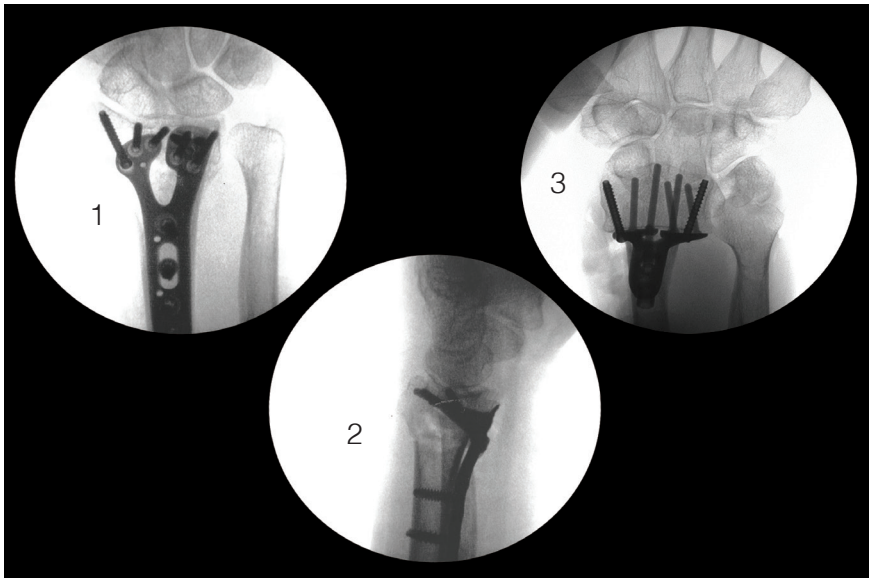

26 FINAL CONFIRMATION

Confirm that ALL pegs and screws have been fully tightened prior to wound closure.

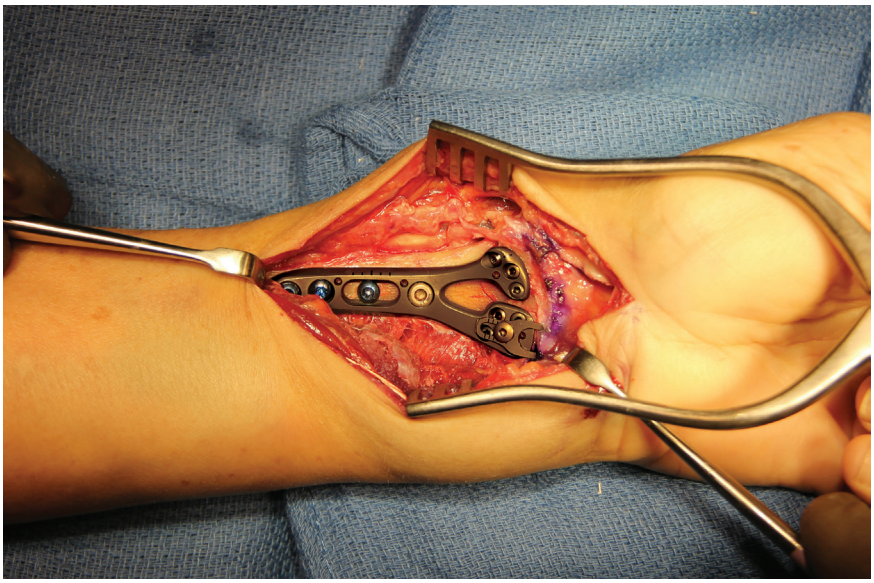


27 OPTIONAL WASHERS

By using a washer, the 2.7mm fully Threaded Non Locking Peg can be used to lag bone fragments when necessary.

Note: The flat side of the washer should be placed on the bone surface.




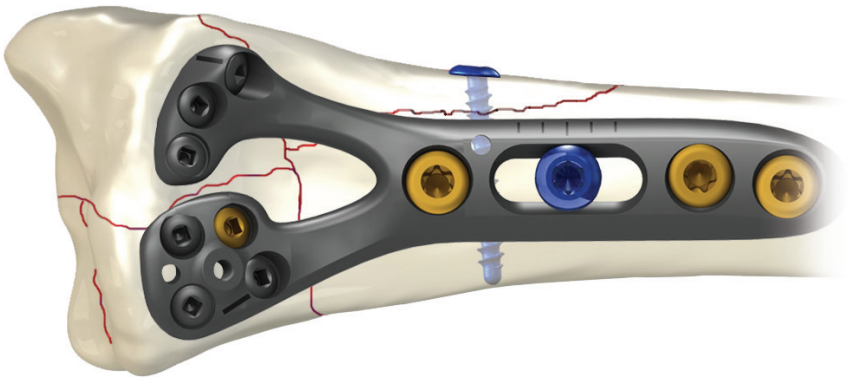

28 BRACHIORADIALIS REPAIR


Repair the brachioradialis in a side-to-side fashion to serve as an attachment point for the PQ muscle.



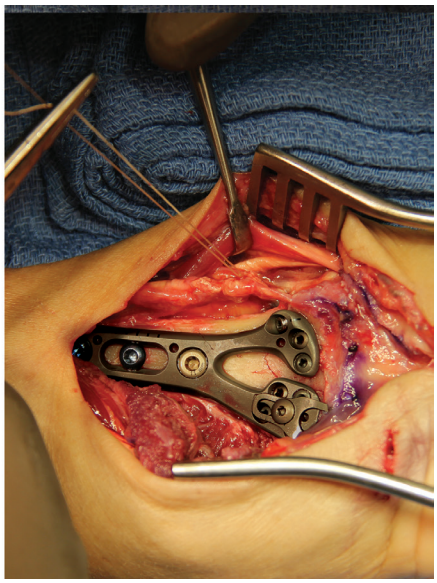


29 TRANSITIONAL FIBROUS ZONE REPAIR


Repair the TFZ in order to cover the distal edge of the GEMINUS plate. This serves to further protect the flexor tendons.

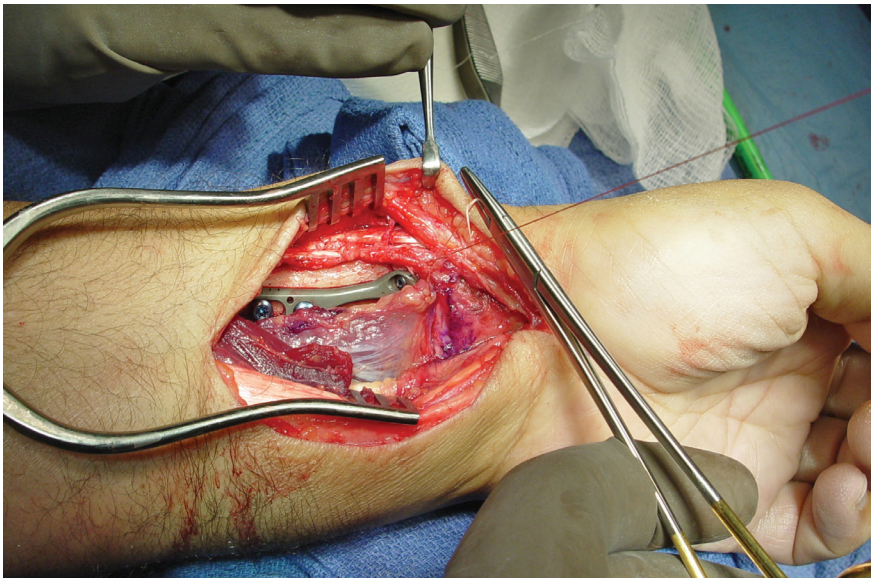

30 PRONATOR QUADRATUS REPAIR


Now suture the PQ muscle to the repaired brachioradialis and TFZ.

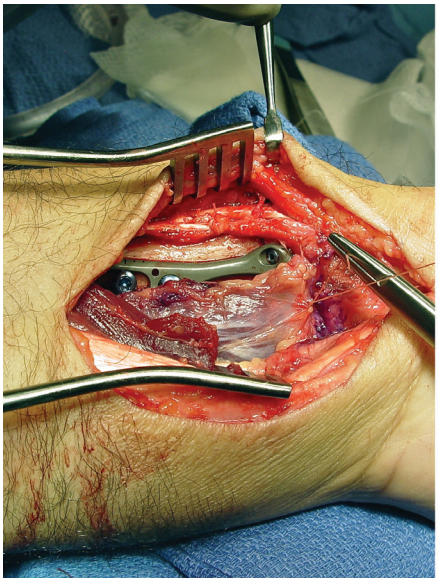


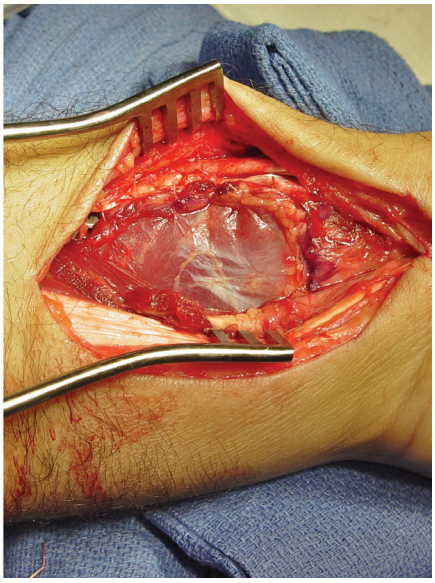

31 FCR TENDON REPOSITIONING

Suture the FCR tendon back to its sheath to support the distal pole of the scaphoid.

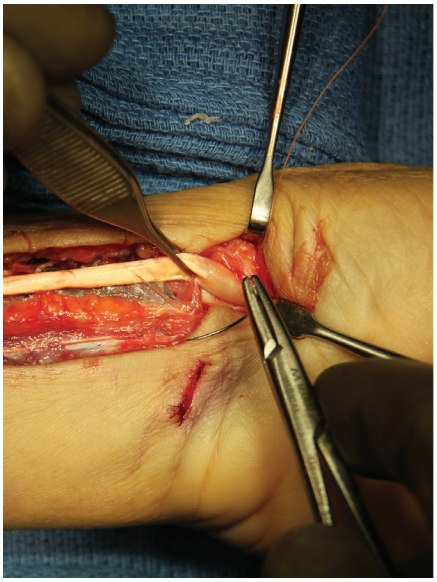

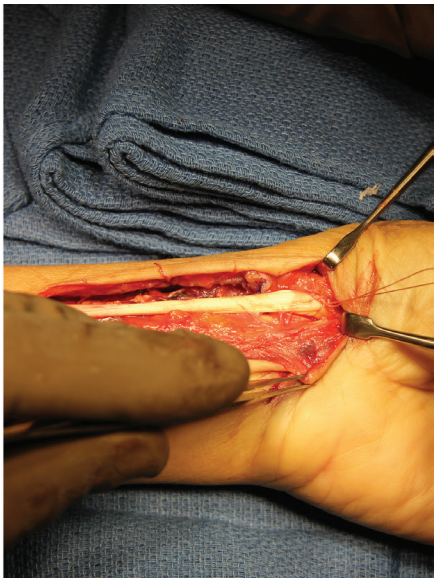

32 WOUND CLOSURE


Close the incision in your normal fashion.




01 PLATE PREPARATION

The PLS is designed to be inserted over a guide wire to assure accuracy.

Remove the desired A.I.M.ing and/or PDG from the plate.

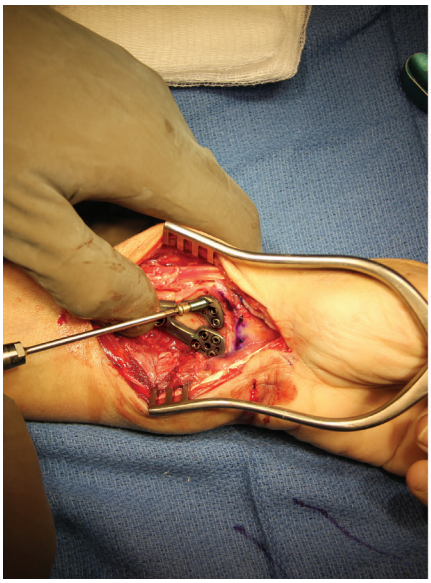

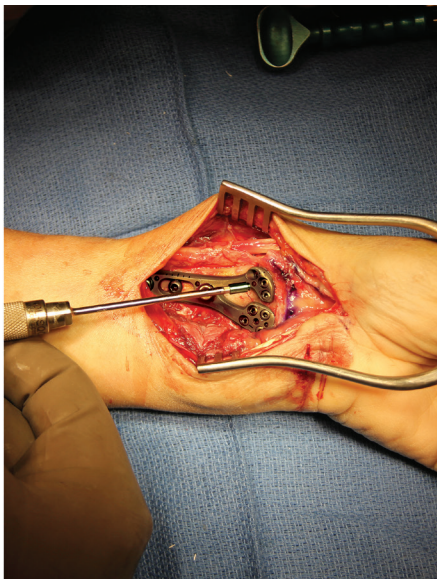



02 ESTABLISHING DESIRED TRAJECTORY

Use the cannulated Initial Driver to secure the PLS A.I.M.ing Guide to the plate.

Insert the gold end of the .9mm K-wire through the PLS A.I.M.ing Guide in the desired trajectory until the far cortex is reached. Confirm the desired placement using fluoroscopy.

Note: The maximum angulation of the PLS should not exceed 10˚ from the trajectory of the respective fixed angle hole.

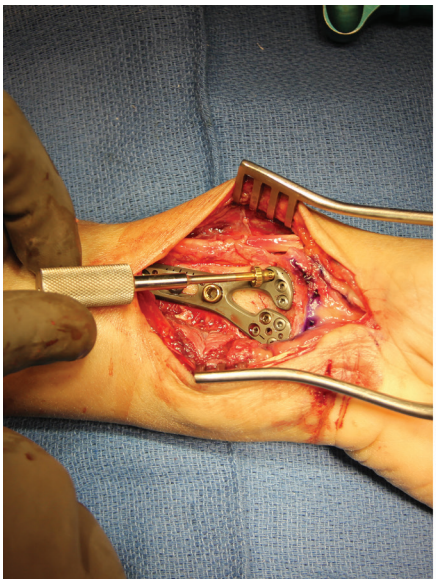

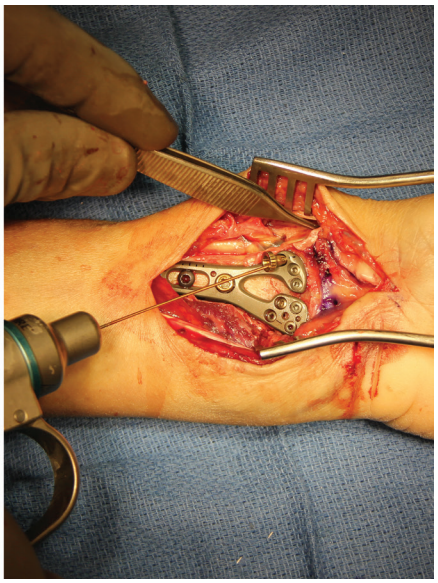



Initial Driver, PLS



PLS A.I.M.ing Guide


K-Wire, 0.9mm


03 MEASURING SCREW LENGTH

Slide the Initial Driver down the K-wire to engage and remove the PLS A.I.M.ing Guide.

Option 1
Confirm that the tip of the K-wire is at the intended position. Slide the PLS Depth Gauge over the K-wire until flush against the plate to measure screw length.

Option 2
The GEMINUS system's Depth Gauge can also be used. However, the 0.9mm K-wire must first be removed then reinserted and proper replacement confirmed using fluoroscopy.

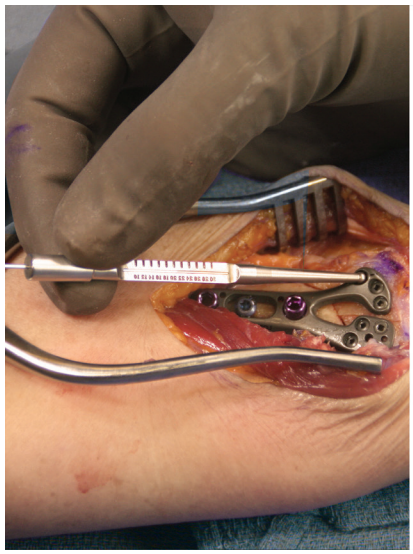

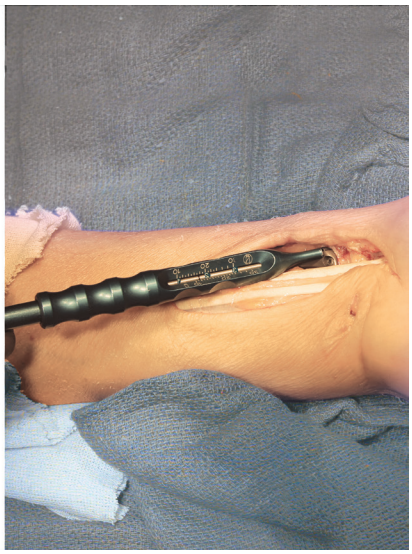




Option 1




Option 2

04 PILOT HOLE PREPARATION

Drill over the K-wire using the 2.0mm Cannulated Drill, then remove it leaving the K-wire in place.

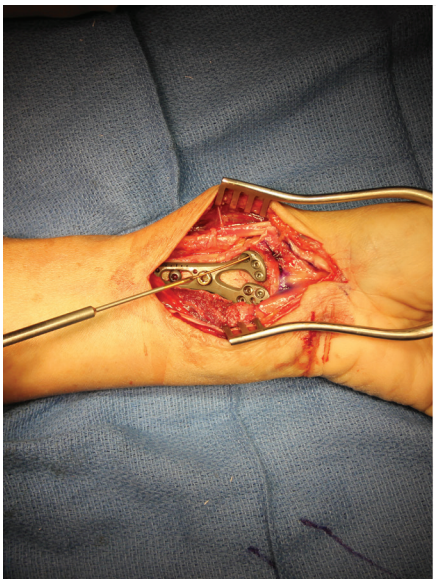

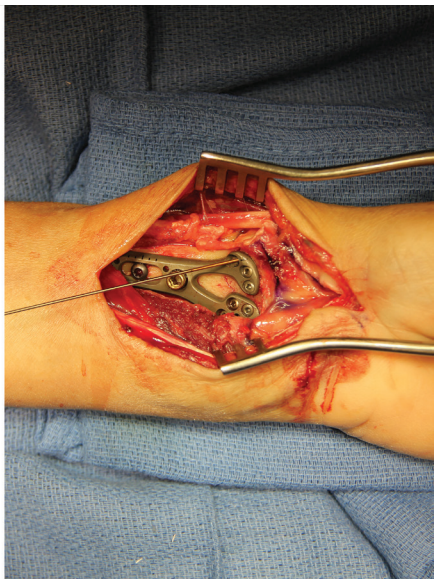




Drill, Cannulated, 2.0mm


05 SCREW INSERTION

Using the Cannulated Initial Driver, insert the appropriate PLS over the guide-wire and into the desired trajectory until the head of the PLS engages the plate.



Initial Driver, PLS

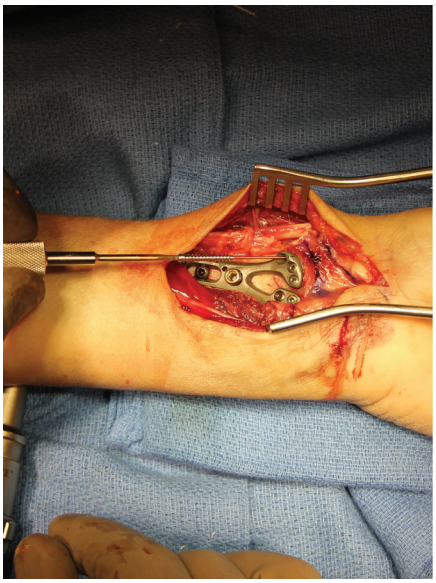

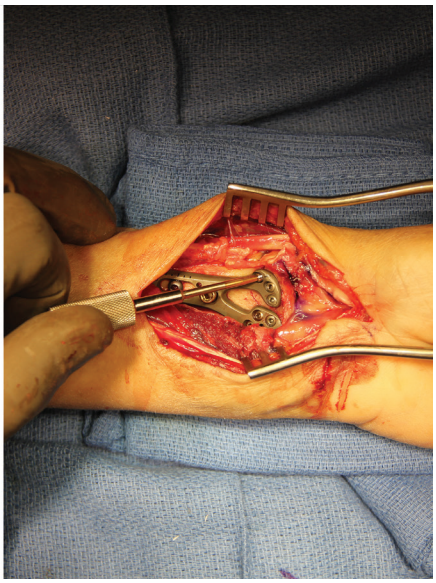


06 LOCKING THE SCREW


Remove the Initial Driver and K-wire.

Using the stronger Non-cannulated PLS Final Driver, be sure to fully seat and lock the PLS into the plate.



Final Driver, PLS

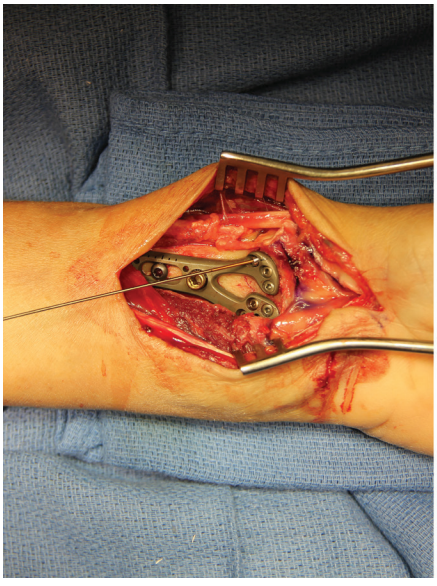


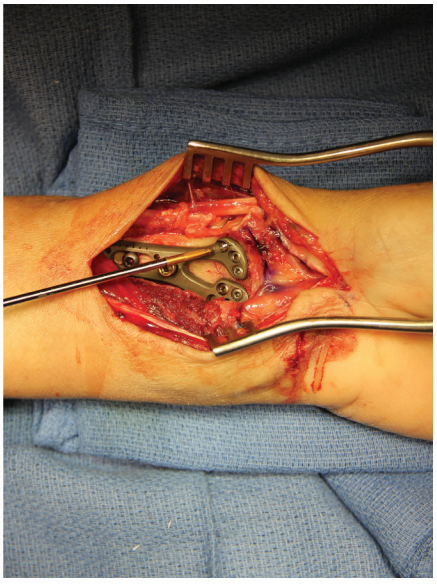

07 FINAL RADIOGRAPHS


Confirm reduction, proper screw length and placement in the AP view (1), a 20˚ elevated lateral fluoroscopic view (2) and by rotating the wrist under fluoroscopy using a tangential view (3).

Warning: Remove ALL PDG's and A.I.M.ing Guides.

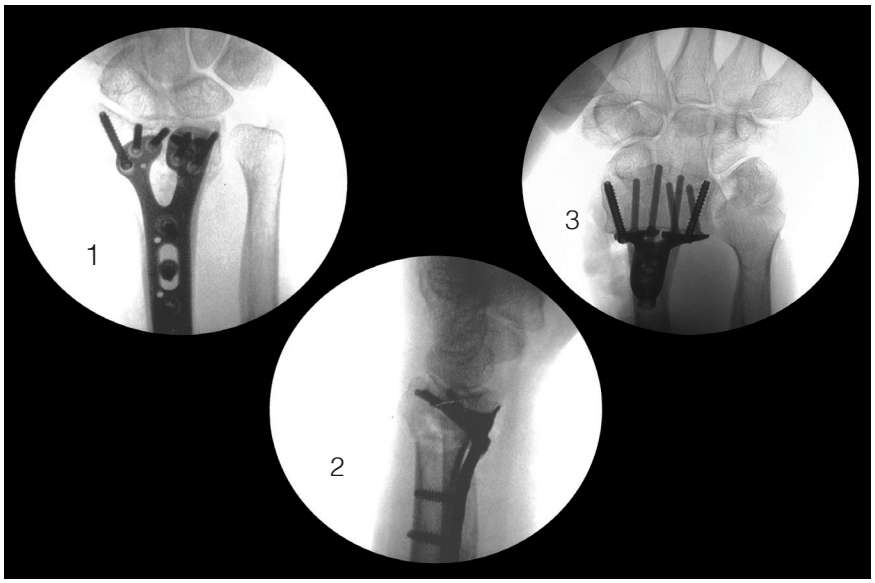

08 FINAL CONFIRMATION


Confirm that ALL pegs and screws have been fully tightened prior to wound closure.

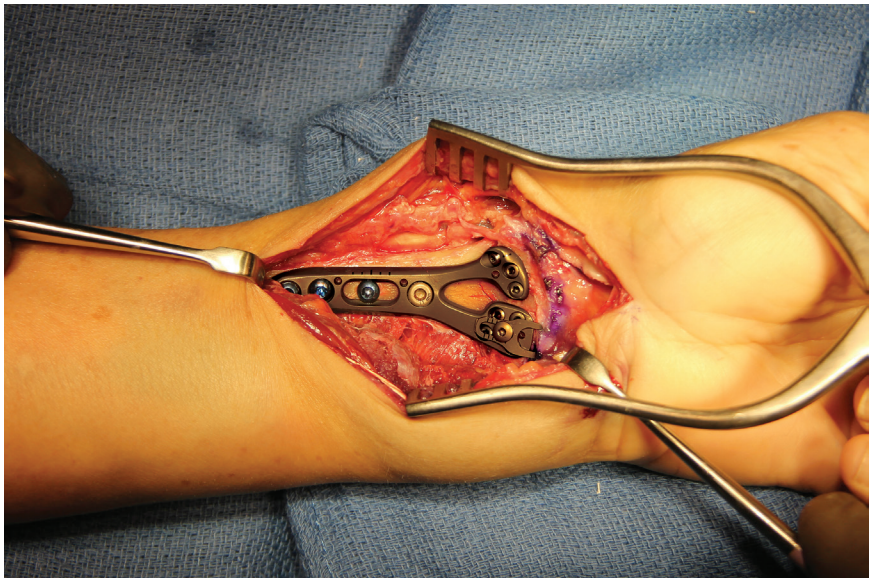

01 GUIDE WIRE PLACEMENT

Advance a 1.6mm K-wire through the central HPE screw hole (A) located on the lunate head of the GEMINUS volar plate.

This K-wire helps to position the Reduction Tool when reducing the volar marginal fragment (VMF).

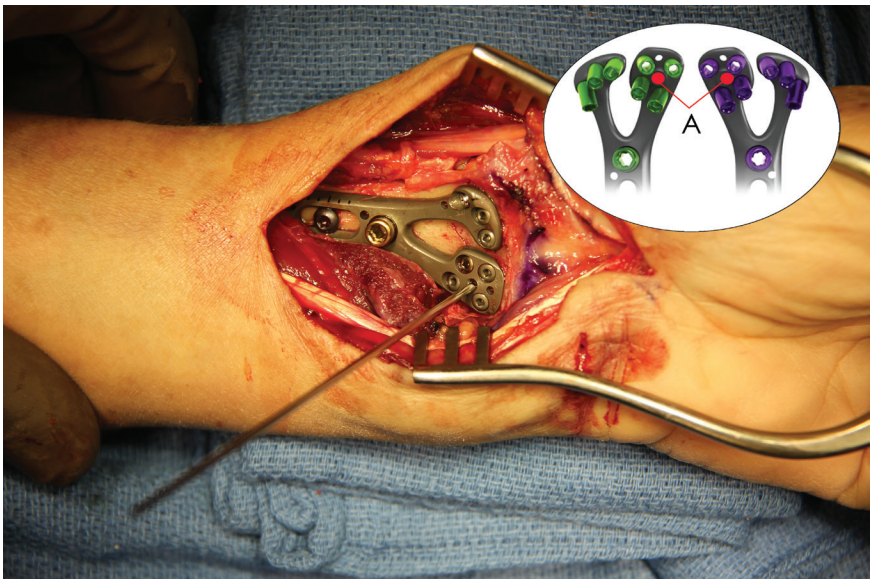

K-wire, 1.6mm

02 REDUCING THE VMF


Slide the slot of the Reduction Tool over the K-wire.

Use the hooked tip of the Reduction Tool to reduce the VMF to the plate.

Note: When properly positioned, the base of the Reduction Tool should be flush to the plate with the handle parallel to the radial shaft.



Hook Plate Reduction Tool

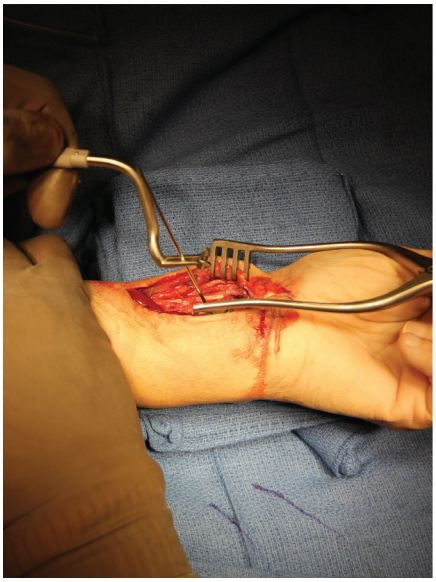





03 PILOT HOLE PREPARATION

While maintaining the reduction, drill a 1.6mm K-wire through both holes of the Reduction Tool.

Leave the K-wire in place within the second drilled hole.

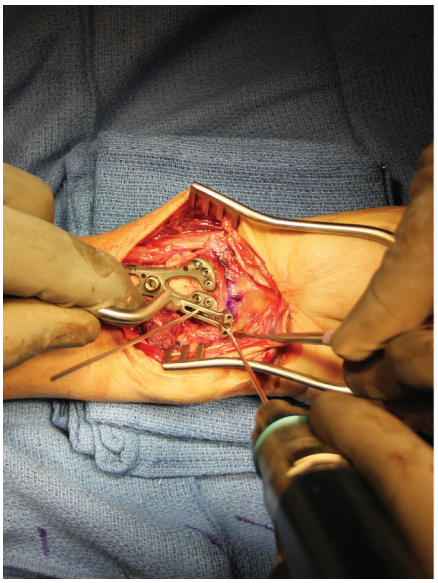

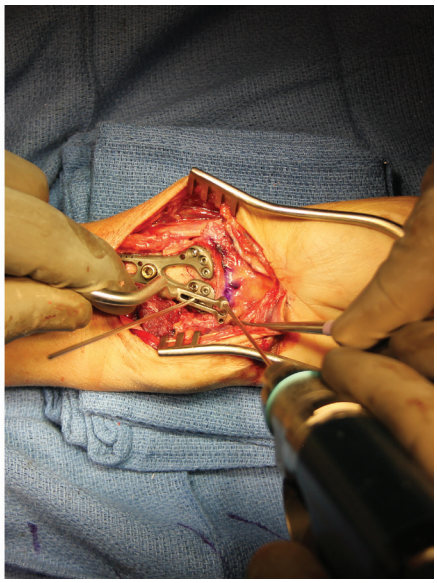

04 CONFIRM REDUCTION

Using fluoroscopy, confirm the reduction, and proper placement of the K-wire 1-2mm proximal to the subchondral plate.

Note: To avoid contact with flexor tendons, the HPE must be applied proximal to and below the watershed line.




05 REDUCTION TOOL REMOVAL


Remove the K-wire from the central Hook Plate Extension screw hole on the plate.

While maintaining the position of the reduced VMF, remove the Reduction Tool by sliding it off of the K-wire.

Note: Take care not to remove the K-wire to prevent VMF displacement.

You can mark the pre-drilled hole to ease visualization.

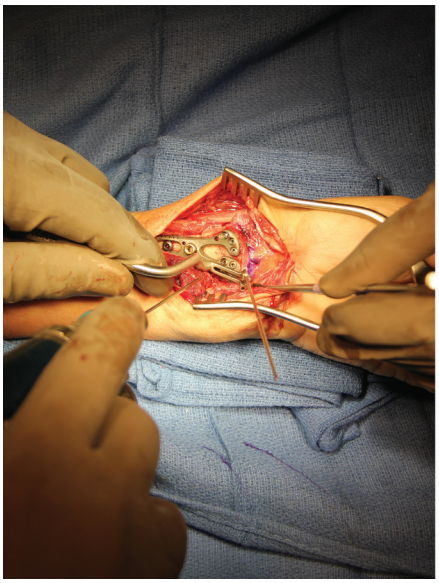

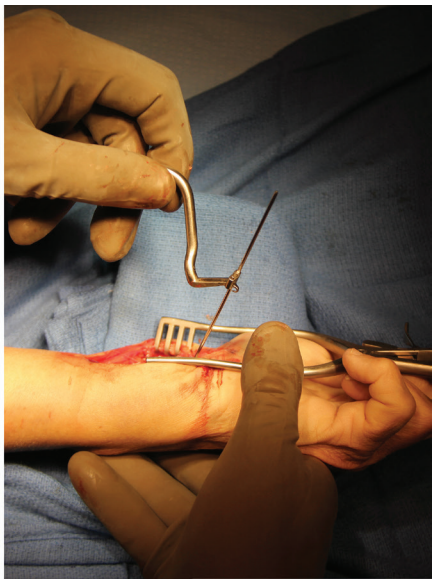

06 HPE PREPARATION


Using a pin cutter, trim the distal half of the HPE leg that corresponds to the remaining K-wire.

Note: Cut the leg at an angle to facilitate insertion (pin cutter not included).



Hook Plate



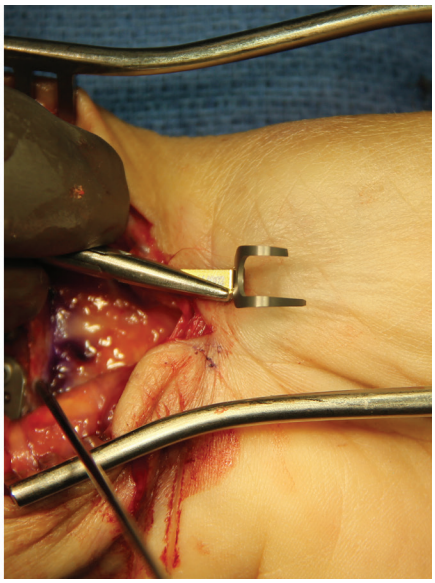



07 HPE INSERTION

Use a needle holder to grip the HPE by the breakaway handling tab.

Insert the long leg into the first pre-drilled hole of the VMF.

Remove the remaining K-wire, then insert the short leg into the now vacant hole.

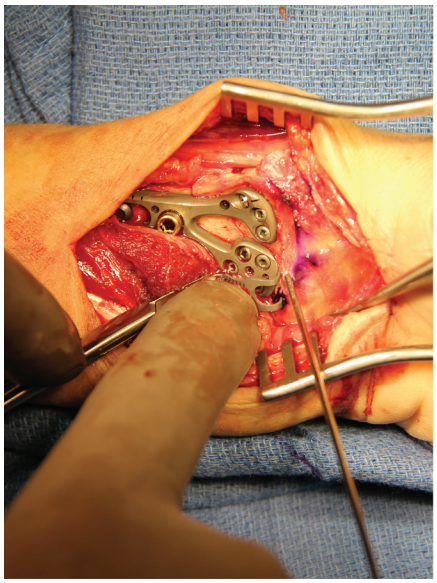

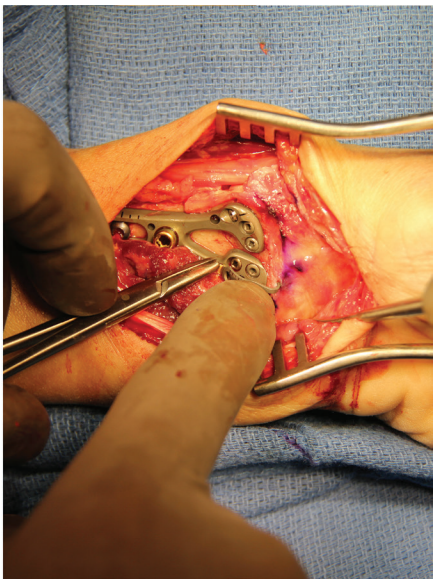



08 LOCKING THE HPE

Lock the HPE to the GEMINUS plate using the Square Tip Driver and an HPE Screw.

Remove the breakaway handling tab by lowering it toward the radius and separating it from the HPE.

Note: Confirm that the HPE Screw is fully secured to the GEMINUS plate.

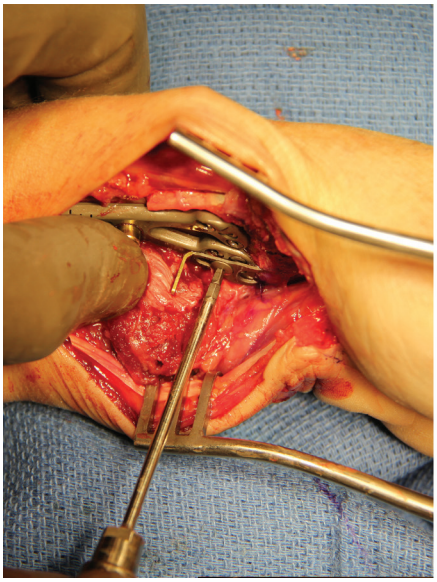

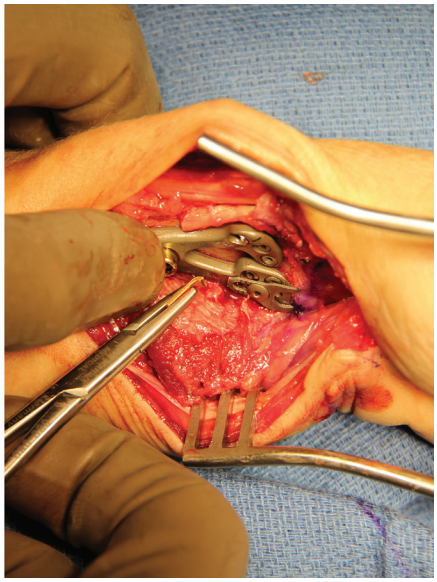



HPE Screw


Driver, Square Tip, 2.0mm

09 FINAL FLUOROSCOPIC CONFIRMATION

Confirm proper placement of the HPE using fluoroscopy.

It should capture the VMF with its legs positioned just beneath the subchondral bone.

Refer to page 17, steps 28-32 for soft tissue repairs and wound closure.

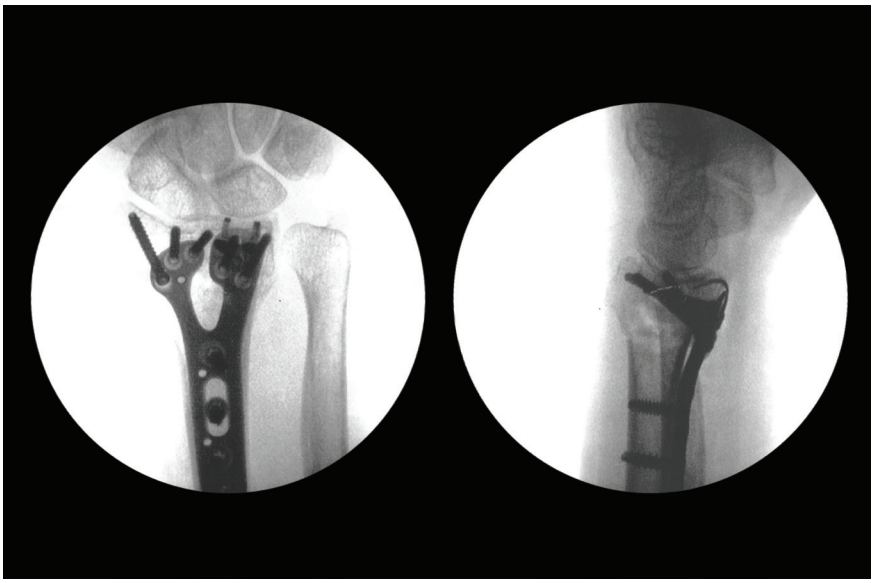

01 GEMINUS XL WITH FREEFIX® TECHNOLOGY


The GEMINUS XL plates are configured with the narrow head width and available in three shaft lengths: 120mm, 160mm, 200mm.

The shaft of the XL plates also incorporates FreeFix® technology, an 8mm threaded slot that provides two differentiating clinical benefits:

1. FreeFix® holes can accommodate both compression or locking screws for plate to bone fixation and dynamic compression.

2. FreeFix® technology provides 1.5mm of dynamic compression.



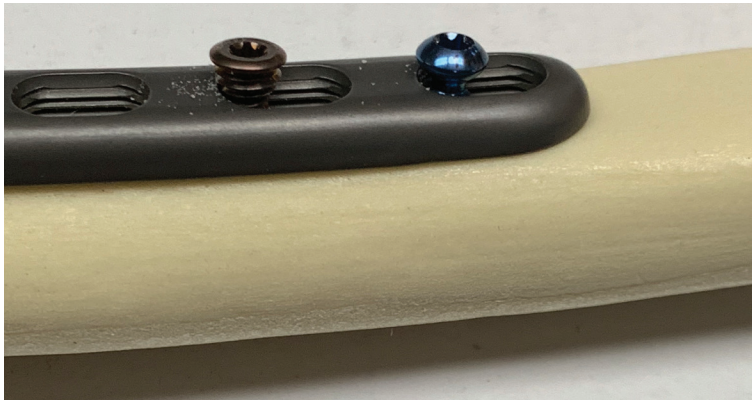



02 FREEFIX® DRILL GUIDE

The FreeFix® drill guide has three drill hole options; the middle hole affixes the plate to bone. Two edge holes allow for dynamic compression of the fracture. Use the drill hole furthest from the fracture to achieve dynamic compression, following AO principles. See chart on page 33 for AO principles regarding dynamic compression.

Using the offset hole furthest from the fracture provides 1.5mm of dynamic compression.

Note: The FreeFix® hole can be drilled free hand if using a compression screw; however, if a locking screw is used, the Drill Guide must be used to ensure the hole is drilled perpendicular to the plate, ensuring the locking screw engages the plate.

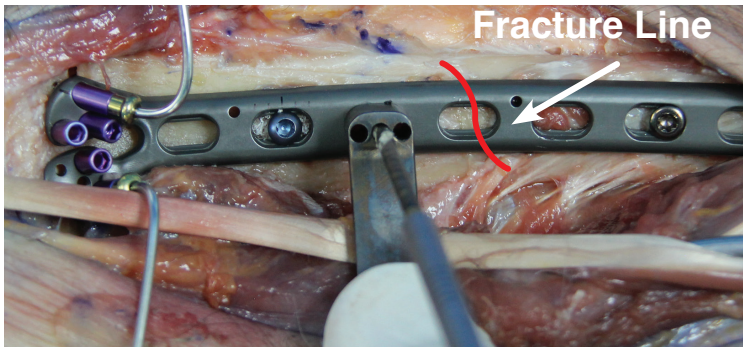

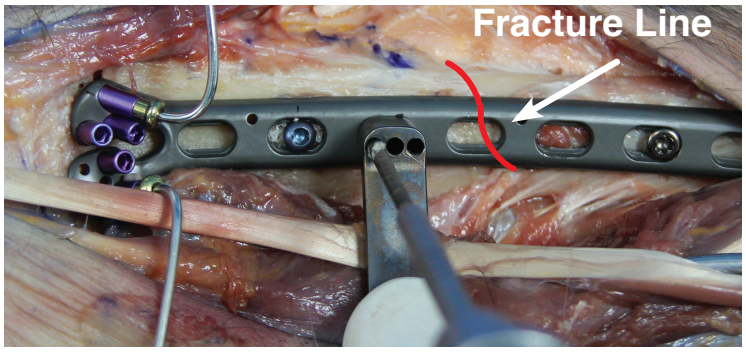


03 FREEFIX® SCREW OPTIONS

The FreeFix® threaded holes accept the 3.5mm compression screws or 3.5mm locking screws.



04 EVALUATION, EXPOSURE AND SURGICAL APPROACH

Radiographically assess the fracture(s), perform steps 1-12 in the main section of this surgical technique guide. (pages 4-9)

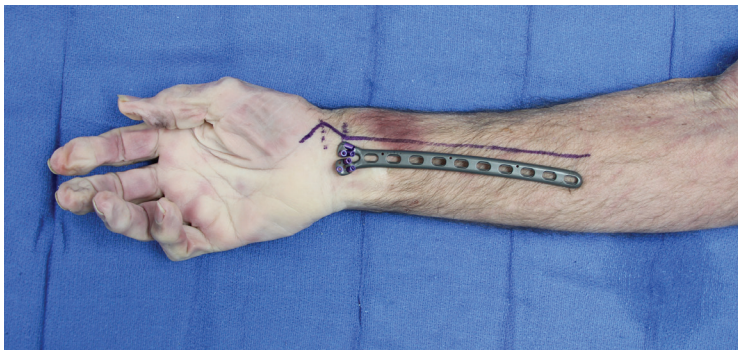







05 INITIAL FRACTURE REDUCTION



Provisionally reduce all fragments.

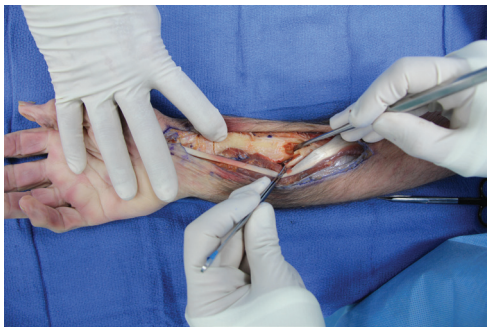

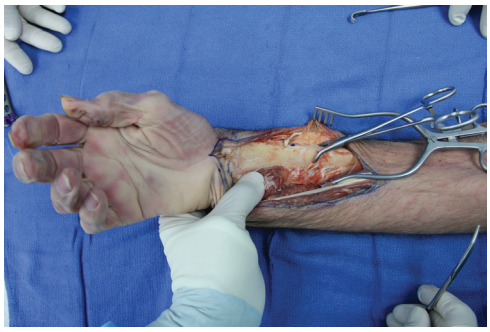


06 DISTAL PLATE PROVISIONAL FIXATION


Perform steps 16-18 in the main section of this surgical technique guide. (pages 11-12)

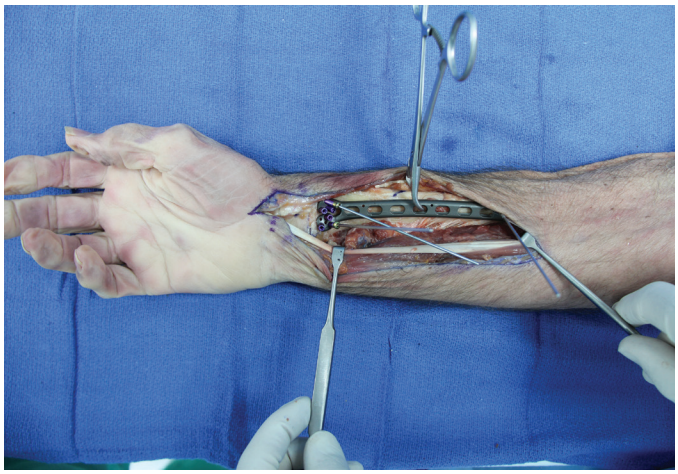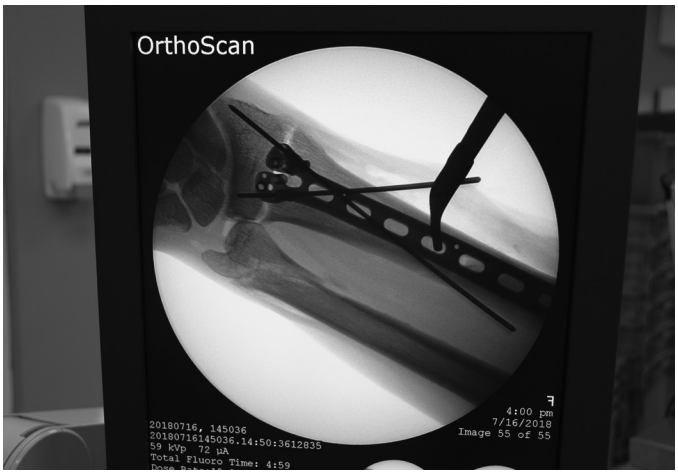07 PROXIMAL PLATE FIXATION (PROVISIONAL)

Secure all proximal fragments to the GEMINUS XL plate using bone clamps or K-wires through the designated holes along the shaft of the plate.



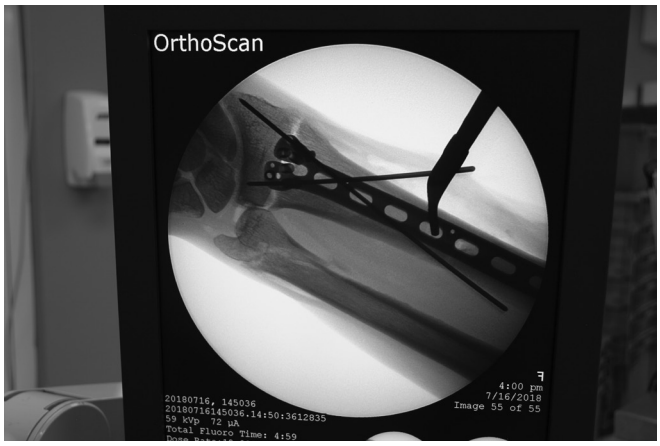

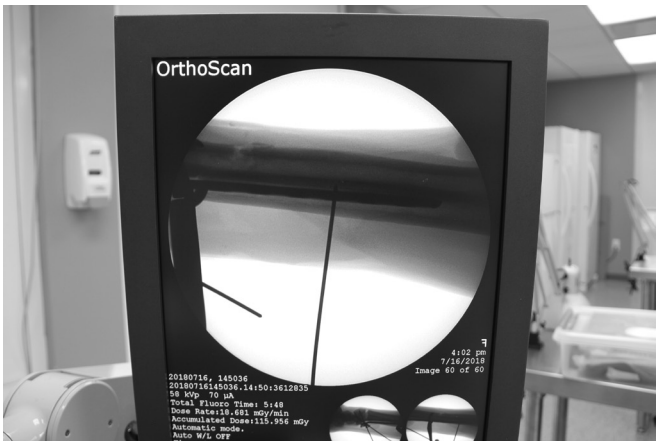
08 PROXIMAL PLATE FIXATION (FINAL)

Seat the FreeFix® Drill Guide in the plate until flush. Using the 2.5mm bit, drill though one of the holes of the Drill Guide to achieve the desired outcome.


Measure the screw length using the Depth Gauge taking note of the appropriate scale.

Insert the appropriate length 3.5mm compression or locking screw using the T-10 driver.

Repeat for all remaining screw holes.

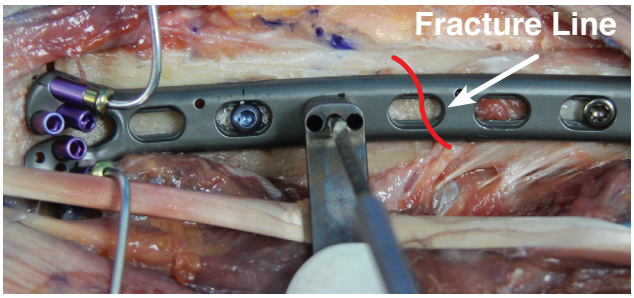


OR

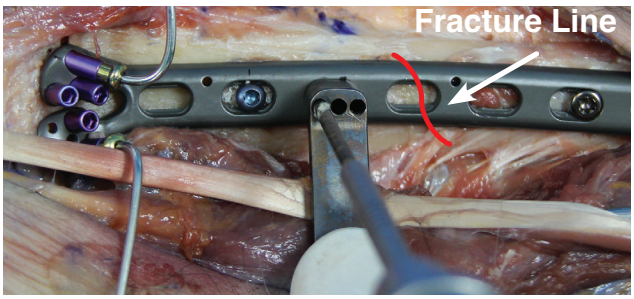

(For dynamic compression)


09 DISTAL PLATE FINAL FIXATION

For distal plate final fixation, refer to steps 19-22 in main section of this surgical technique guide. (pages 13-14)

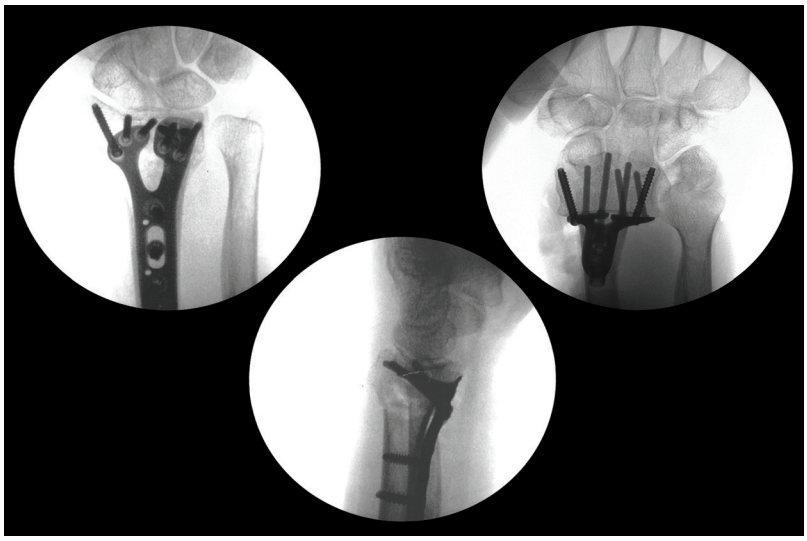

AO REFERENCE CHART FOR DYNAMIC COMPRESSION


After insertion of one compressing screw, it is only possible to insert one further screw with compressing screw against the side of the screw hole and prevents further movement. When the second screw is tightened, the first has to be loosened to allow the plate to slide on the bone, after which it is retightened.

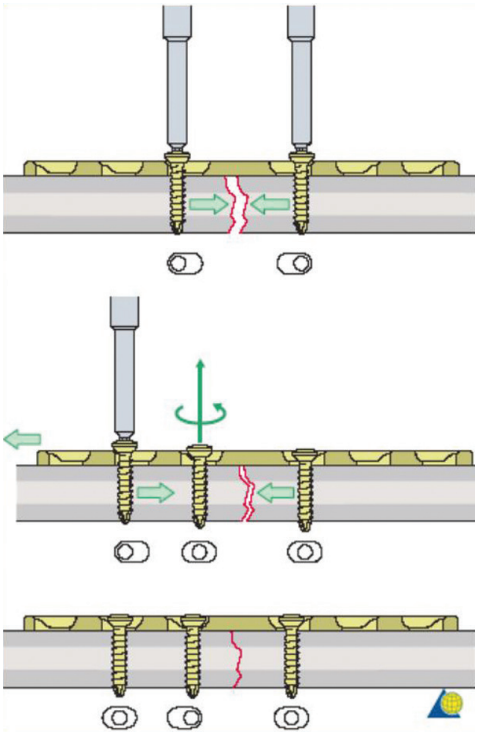

01 ESTABLISHING VOLAR TILT

Insert the blunt end of a .062 K-wire through the wrist capsule at the level of the interfossa sulcus.

Confirm proper placement parallel to the joint using a 20^0-30^0 elevated lateral fluoroscopic view.

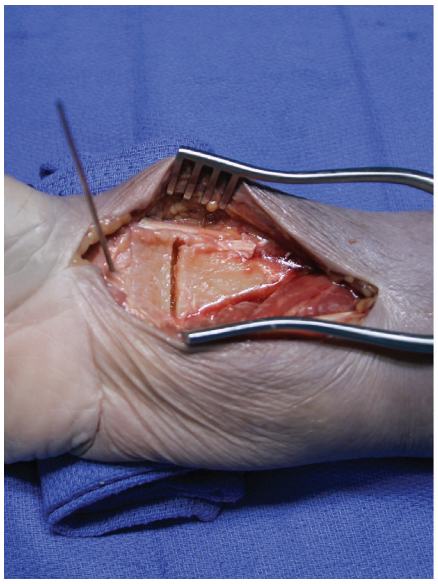





02 PLATE POSITIONING

Place the plate approximately 2mm proximal and parallel to the watershed line, centered on the distal fragment. This will correct the coronal plane deformity.

Elevate the shaft of the plate with respect to the distal fragment to the estimated volar tilt.

Insert the alignment K-wire through the distal hole of the plate. Confirm it is positioned parallel to the joint, and that proper volar tilt has been achieved.

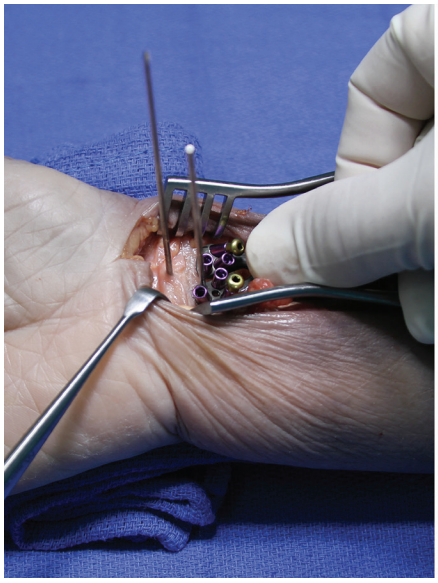

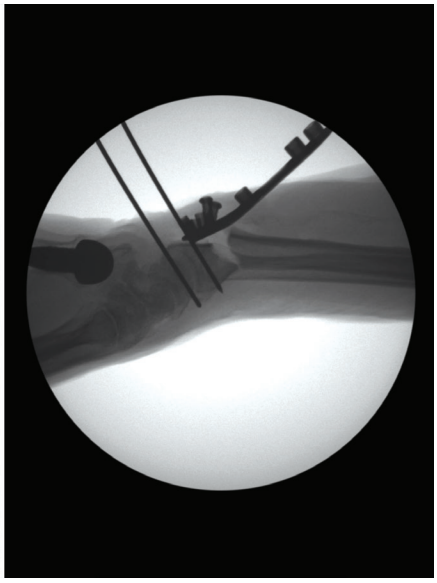



03 PROVISIONAL DISTAL FIXATION

Insert a K-wire into the A.I.M.ing guides through the most ulnar and radial holes.

Confirm proper placement of the K-wires referencing page 12, steps 17-18.

After the GEMINUS plate has been fixed to the distal fragment, remove the distal most K-wire used to reference the joint line.

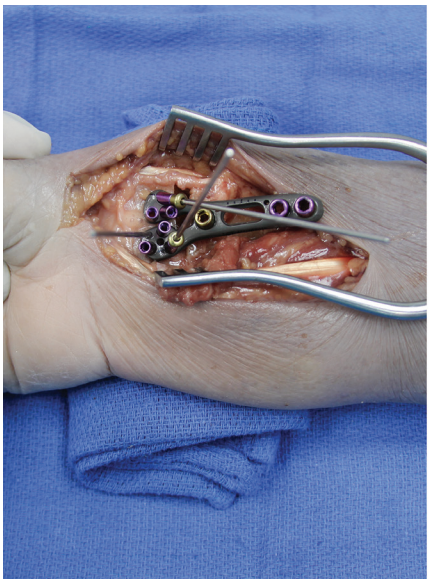

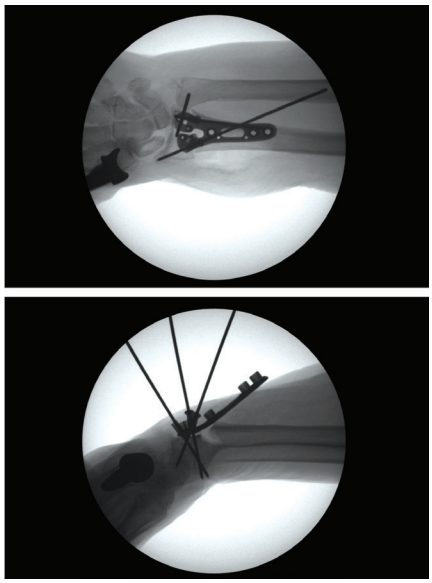


04 FINAL DISTAL FIXATION

Secure the GEMINUS plate to the distal fragment as previously described on page 13, in the main section of this surgical technique guide.

Confirm reduction and proper peg placement in the AP view (1), a 20˚ elevated lateral fluoroscopic view (2)
and by rotating the wrist under fluoroscopy using a tangential view (3).


Warning: Remove ALL PDG's and A.I.M.ing Guides.



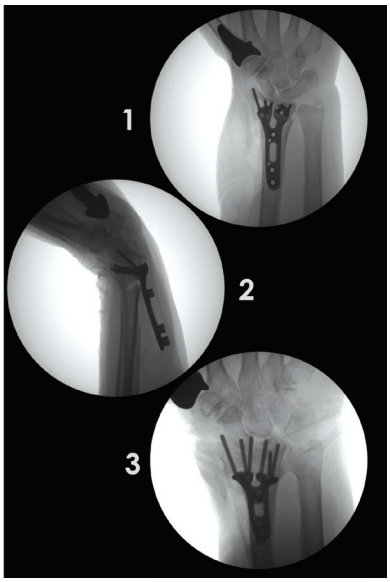


05 RESTORING VOLAR TILT

Lower the shaft of the GEMINUS plate to the radial shaft to reduce the fracture.

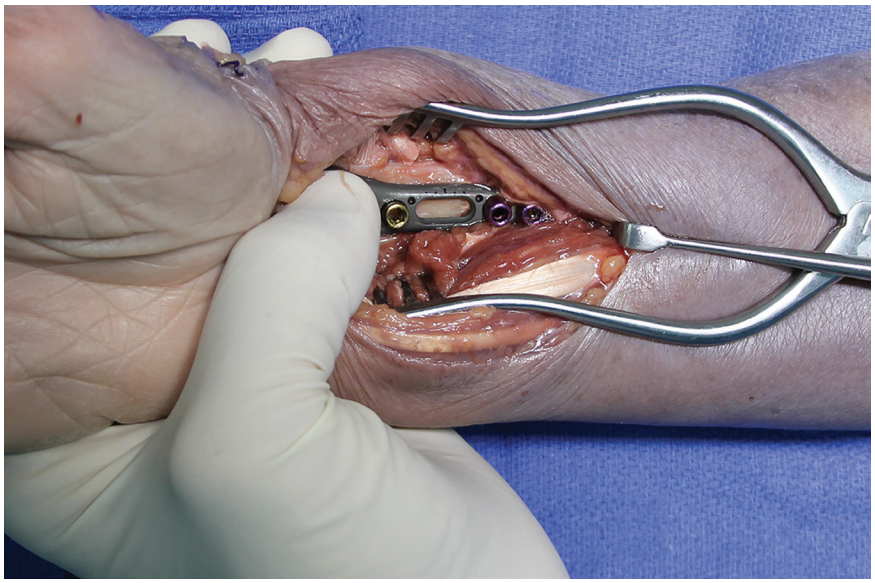

06 PROXIMAL PLATE FIXATION


Secure the shaft of the GEMINUS plate to the radial shaft as previously described in steps 15 and 24 in the main section of this surgical technique guide.

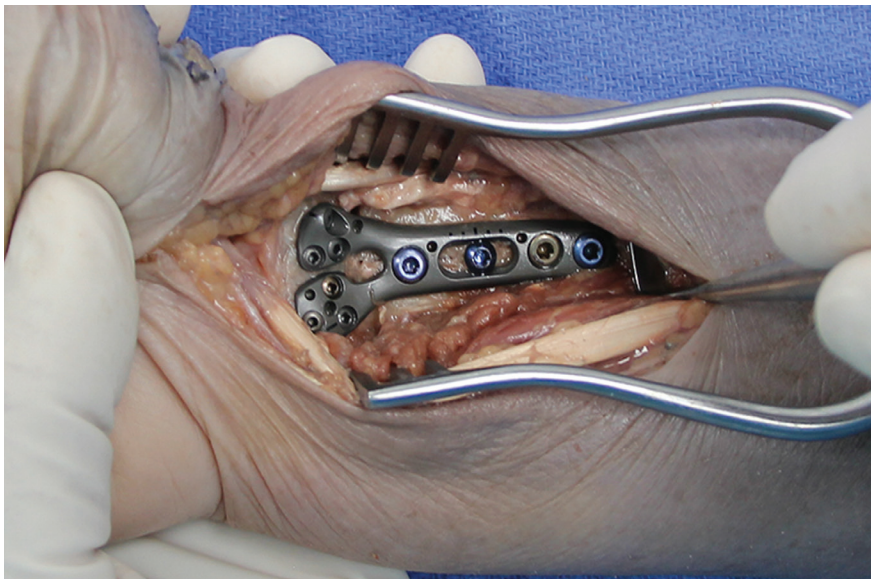

07 FLUOROSCOPIC CONFIRMATION

Confirm that proper radial length, inclination and volar tilt have been achieved using fluoroscopy.

Close the wound as described starting on page 17, steps 28-32 of the main section of this surgical technique guide.

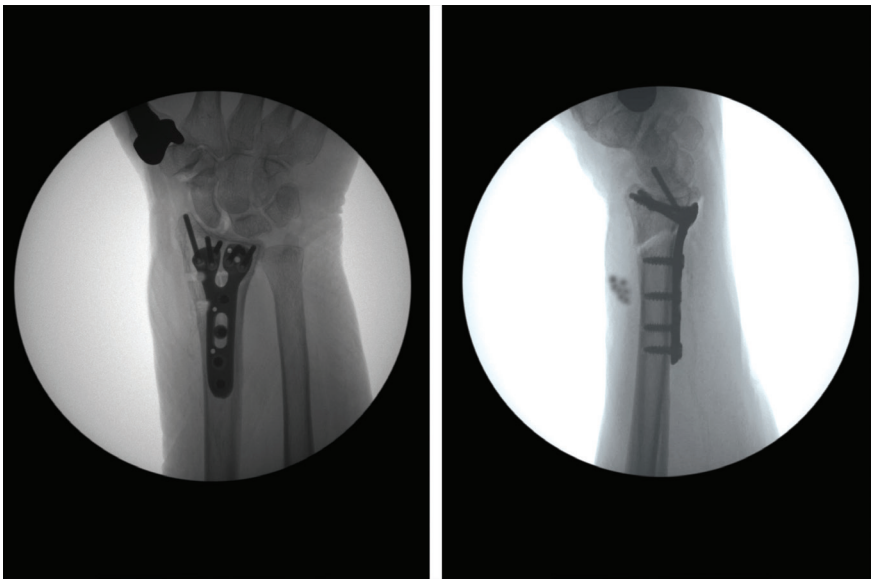

01 DRILL BLOCK SELECTION

There are six reusable GEMINUS Drill Blocks that are size and side specific to each of the GEMINUS plates with gold PDG's in the shaft.

NOTE: The Drill Blocks are not compatible with plates having more that 4 holes in the shaft.

The Blocks are not compatible with Plates with a Radial Hook Plate Hole.

Drill Blocks may not be used if the plate has been contoured.

On the narrow Drill Block, the proximal radial hole on the lunate side accepts the 2.0mm drill directly and the drill guide is not needed.




02 DISTAL PDG REMOVAL

Using the Peg Driver, remove all of the PDG's from both heads of the plate.

Select the appropriate Drill Block for the plate being used.

Align the Drill Block flush to the head of the plate, then secure it by tightening the captive drill guide using the square tip driver.



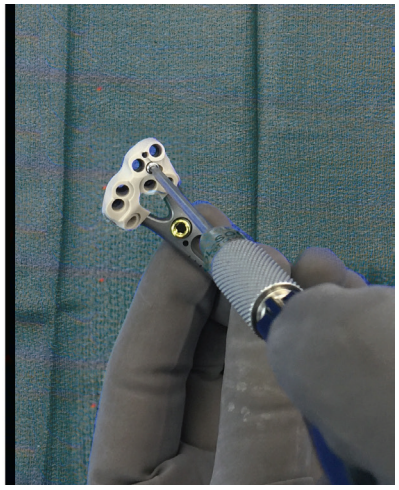



Driver, Square Tip 2.0mm


03 PLATE POSITIONING


Secure an A.I.M.ing Guide into the most proximal ulnar hole of the lunate head and most radial hole on the scaphoid head.

Refer to pages 11-12, steps 15-18 in the main section of this surgical technique guide for proper plate positioning and provisional fixation.



Drill Block, A.I.M.ing Guide, 1.6mm
(Located in the Drill Block Module)

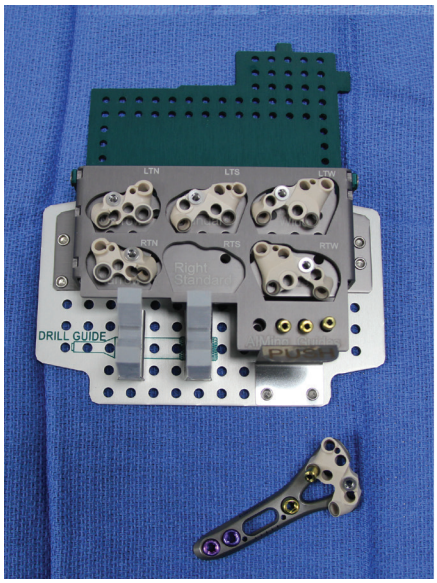

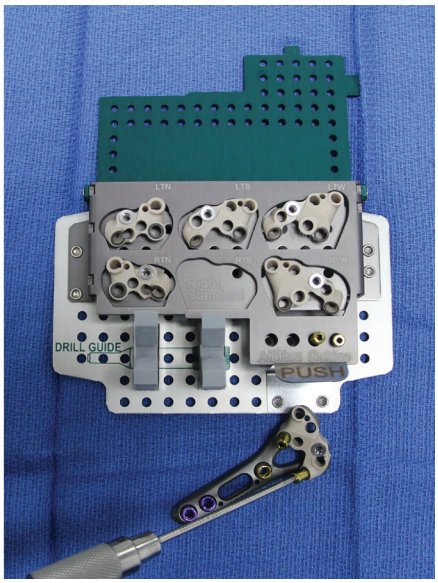


04 PILOT HOLE PREPARATION


Secure the 2.0mm Thread-in Drill Guide into the most proximal medial hole on the lunate side of the Drill Block.

Using the 2.0mm bit, drill through the Thread-in Drill guide.



Thread-in Drill Guide, 2.3mm

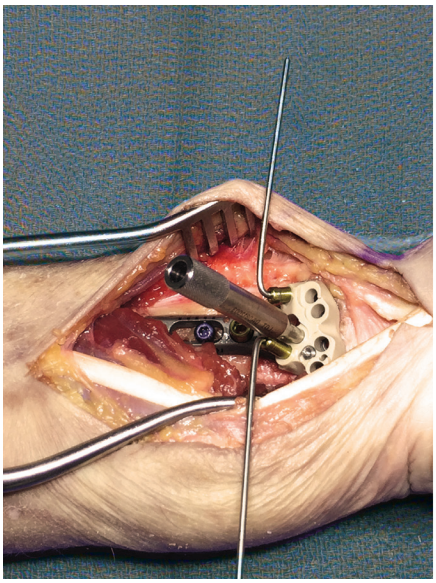

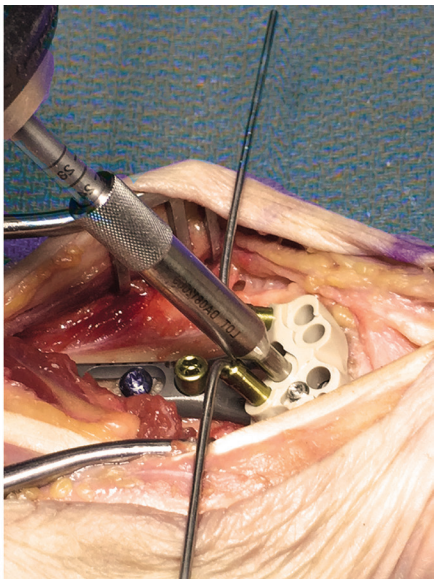



05 MEASURING SCREW LENGTH

Determine the proper screw length by reading the measurement directly from the drill (1).

You can also remove the Thread-in Drill Guide and measure the screw length using the appropriate scale on the Depth Gauge (2).

Note:
The scale with the symbol
is used with the optional Drill Blocks.

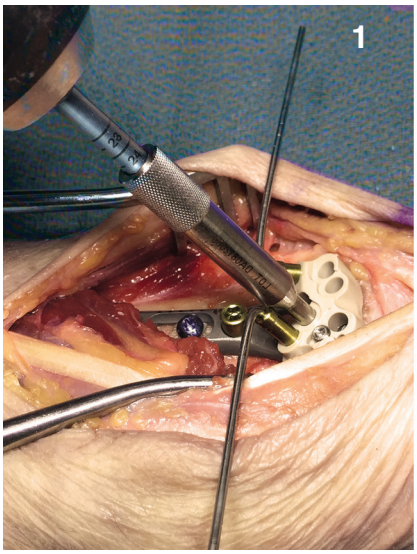

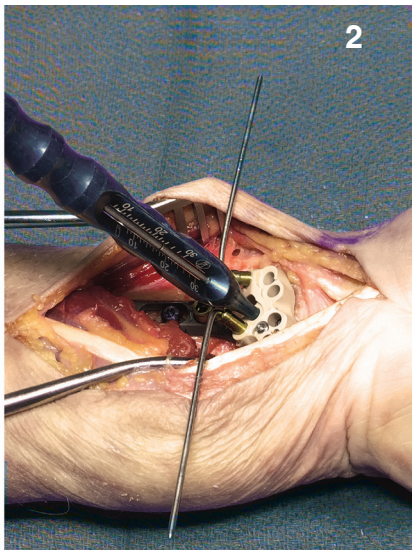




06 DISTAL FRAGMENT FIXATION

Refer to page 13 in the main section of this surgical technique guide for distal fragment fixation.



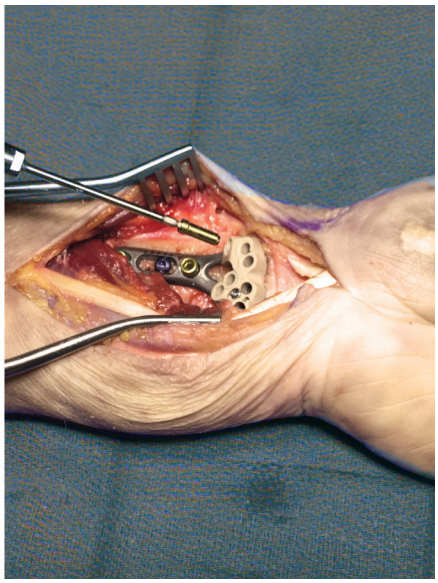



07 FINAL DISTAL FRAGMENT FIXATION

Using the peg driver, remove the Drill Block from the plate.

Prepare the final distal hole of the GEMINUS plate.

For proximal plate fixation and wound closure, refer to the main section of this surgical technique guide, starting on page 15, steps 24-32.

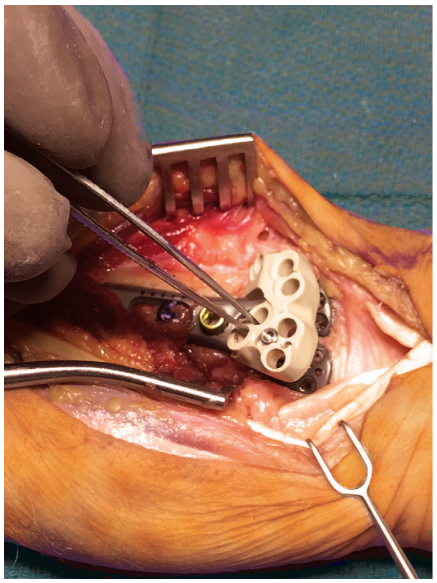

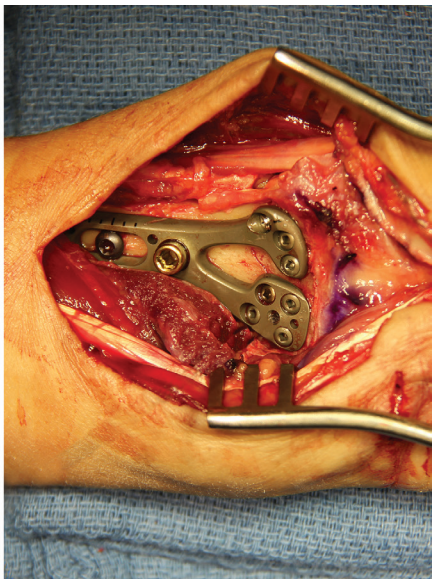

01 FRACTURE EXPOSURE

Expose then debride the fracture.

Reduce the fragment(s) and assess for proper plate positioning.






02 PROTEAN PLIER FEATURES

The PROTEAN plates are designed to be contoured using proprietary Bending Pliers either on the back table or in-situ after plate application.

The plates incorporate a beveled edge that allow for the Bending Pliers to securely grip the plates.

Manipulation can easily be achieved in all three planes at the level of the inter-node sections of the plates.

PROTEAN plates incorporate a unique design:

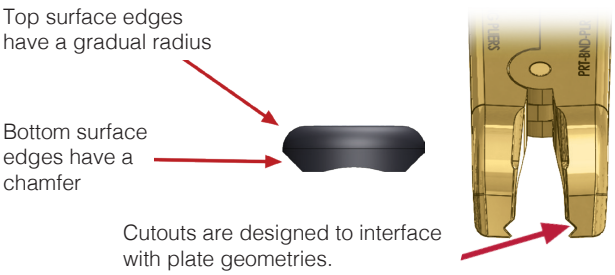

PROTEAN plate benders feature a unique jaw design:




Adapts to plates w/ PDG's




Adapts to plates w/ Thread-In Drill Guides

03 PROTEAN PLATE FEATURES


PROTEAN Fragment Plate, Y - Straight

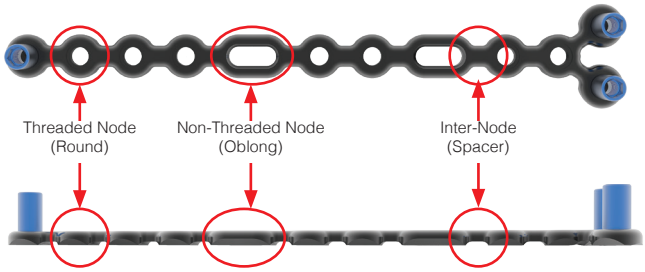


PROTEAN Fragment Plate, Double Hockey Stick

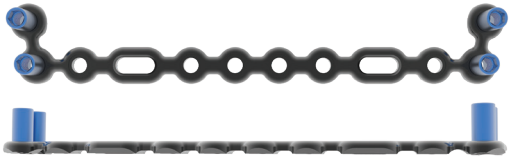

PROTEAN Fragment Plate, Distal Ulna

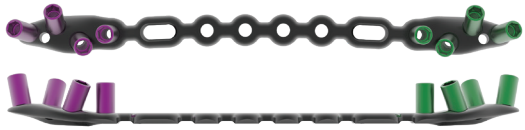

PROTEAN Fragment Plate, Central Column

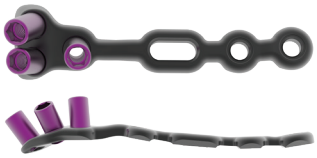

PROTEAN Fragment Plate, Radial Column



PROTEAN Plates:

- Are malleable in three planes
- Accept PDG's or thread-in drill guides
- Accept all screw options

04 PLATE MANIPULATION

To properly contour or cut a plate, securely grip the plate at any two nodes (round or oblong) using the Bending Pliers and shape the plate as intended.

A. Vertical Plane: Secure the pliers to any two nodes for bending up to 30^0.


B. Horizontal Plane: Secure the pliers to any two nodes for bending up to 5^0.

C. Transverse Plane: Secure the pliers to any two nodes for bending up to 45^0.

Note: Do not exceed the respective maximum bend angles as described above.

D. Cutting to length: Bend in continuous motion (undersurface to undersurface) past 120^0.


Warning: Bending may weaken or break the plate. Be sure to inspect the plate for damage prior to use.

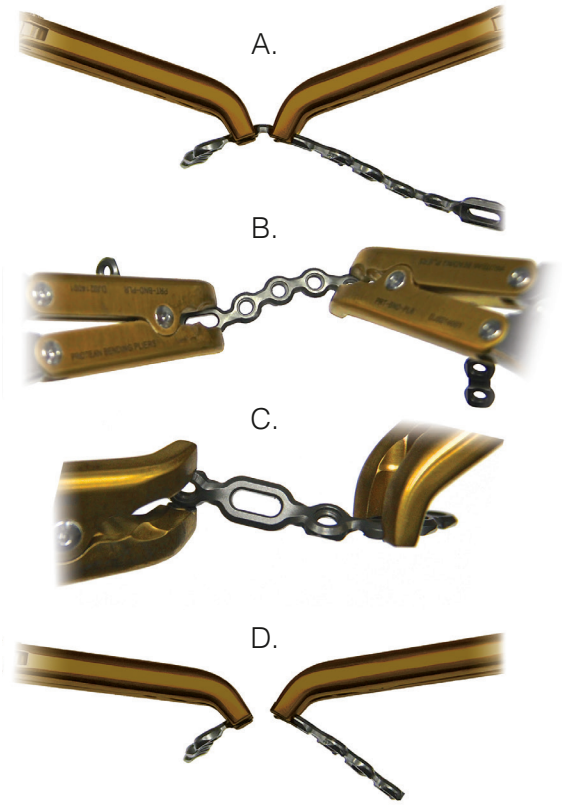


05 PROVISIONAL PLATE SIZING

Position the plate to span the fracture site, then measure and cut to the proper length.


Now provisionally contour the plate to match the anatomy using the Bending Pliers.

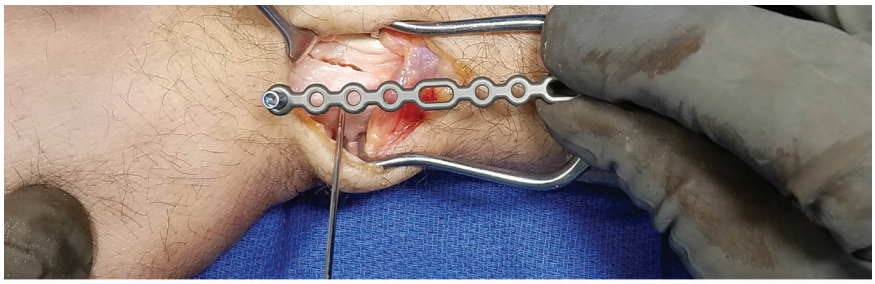


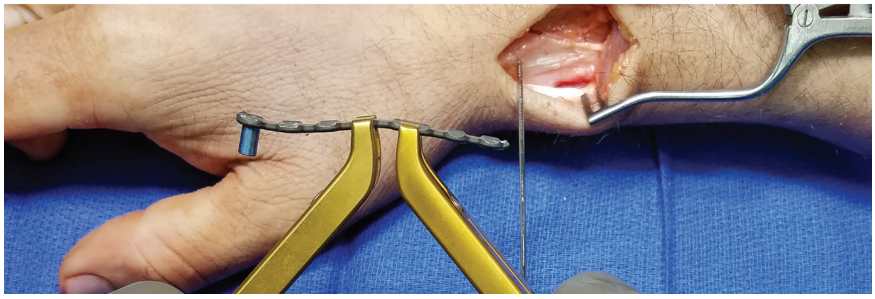

06 LOADING A.I.M.ING GUIDES

Using the Peg Driver, secure A.I.M.ing Guides to the PDG, then use K-wires to stabilize the fragments.

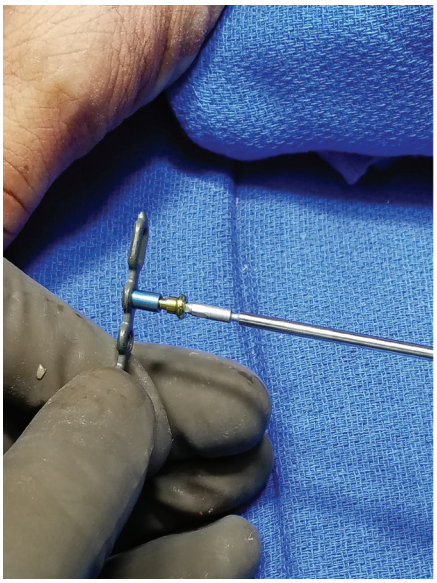

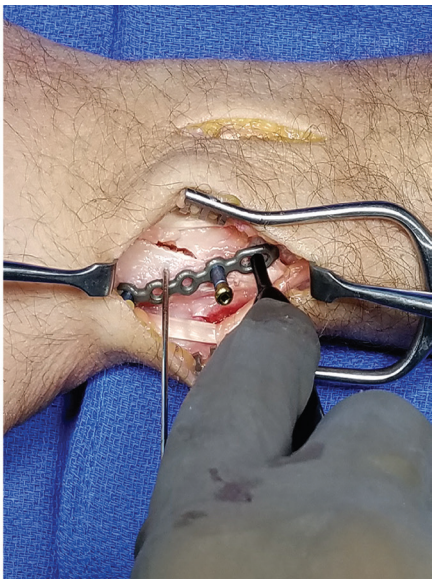


07 PROVISIONAL PLATE FIXATION


Position the Plate to span the fracture line.

Using the 2.0mm bit, drill through an oblong node of the plate.



Drill, 2.0mm x 40mm

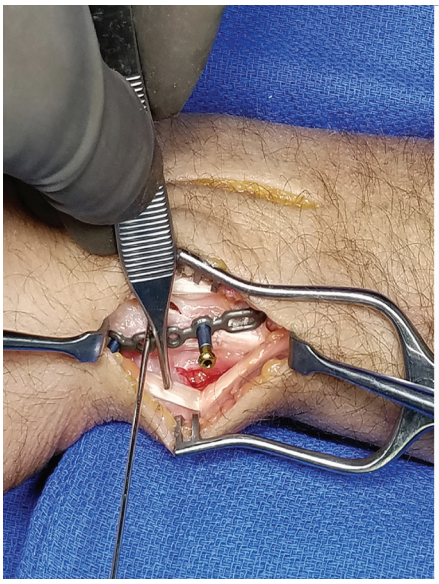

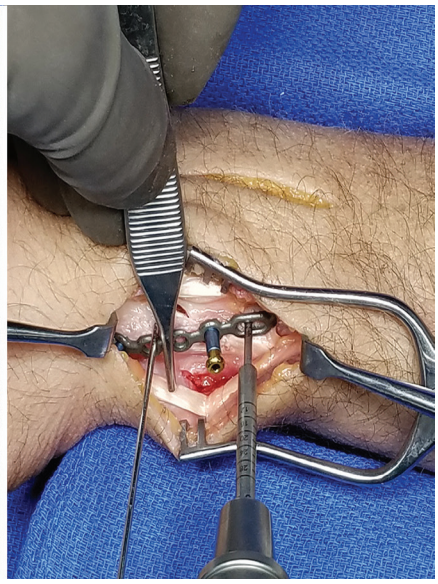

08 SECURING THE PLATE

Measure the screw length using the Depth Gauge.

Now insert a 2.7mm fully Threaded Peg (non locking).



Threaded Peg, Non Locking





09 IN-SITU PLATE CONTOURING

Adjust the plate's position, then contour the plate as needed to match the anatomy using the Bending Pliers.


Note: Be sure to securely hold the plate at the nodes with the Bending Pliers.



10 FINAL FRACTURE REDUCTION

Secure the plate to the fragment(s) using a 1.6mm K-wire through the A.I.M.ing Guides.

Note: Confirm proper placement using fluoroscopy.

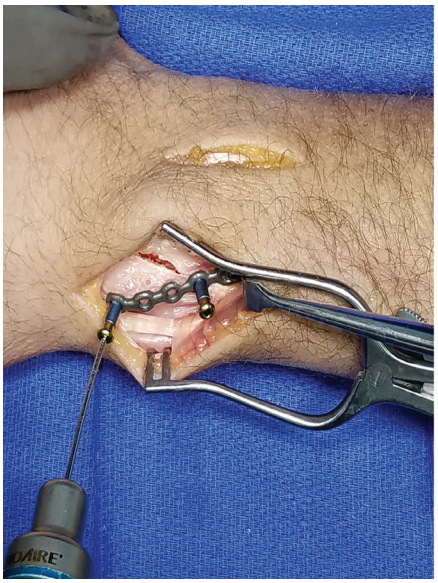




11 DRILLING THROUGH THREAD-IN DRILL GUIDE

If drilling a fixed angle screw through a node that does not have a PDG, secure the 2.0mm Thread-In Drill Guide to the round node.

Drill through the guide using the 2.0mm bit, then measure the screw length directly from the marked drill bit.

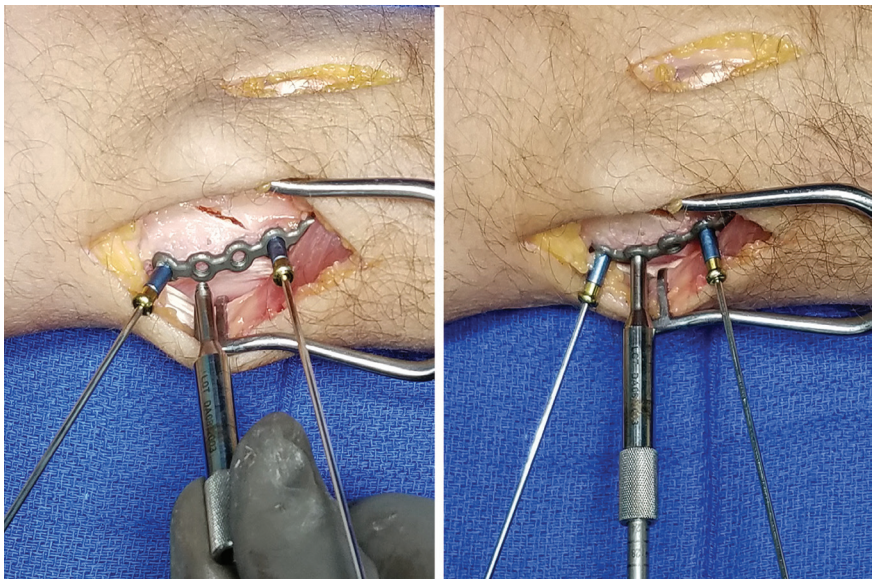




Thread-In Drill Guide, 2.0mm

12 SCREW INSERTION

Remove the Thread-In Drill Guide.

Now insert the appropriate length 2.3mm threaded screw (locking) or a 2.7mm High Compression screw.

Repeat the previous steps for the remaining screw holes.

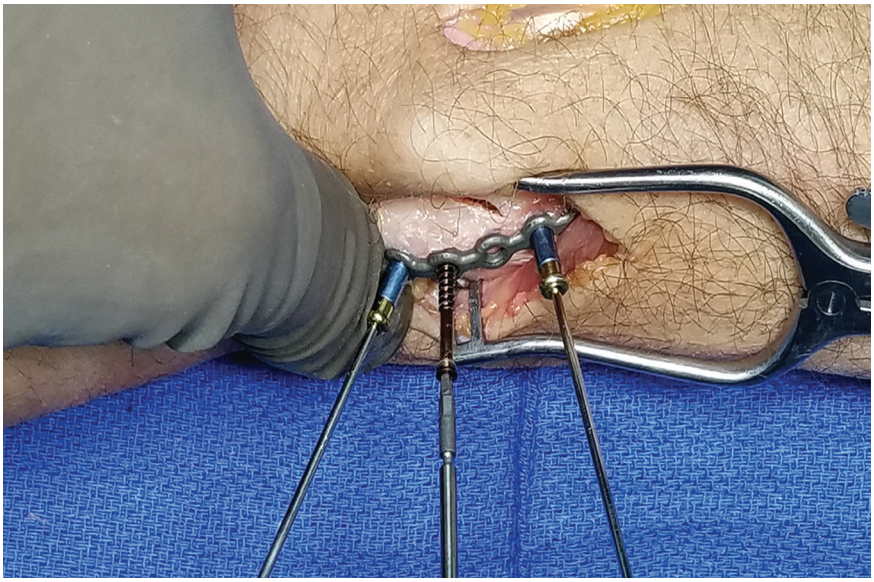



Threaded Peg, Locking



High Compression Locking Peg

13 DRILLING THROUGH THREAD-IN DRILL GUIDE


If present, remove the A.I.M.ing and PDG using the Peg Driver.

Insert the PLS A.I.M.ing Guide into the desired node using the PLS Initial Driver.


Note: The maximum angulation of the PLS should not exceed 10˚ from the trajectory of the respective fixed angle hole.



Initial Driver, PLS




PLS A.I.M.ing Guide

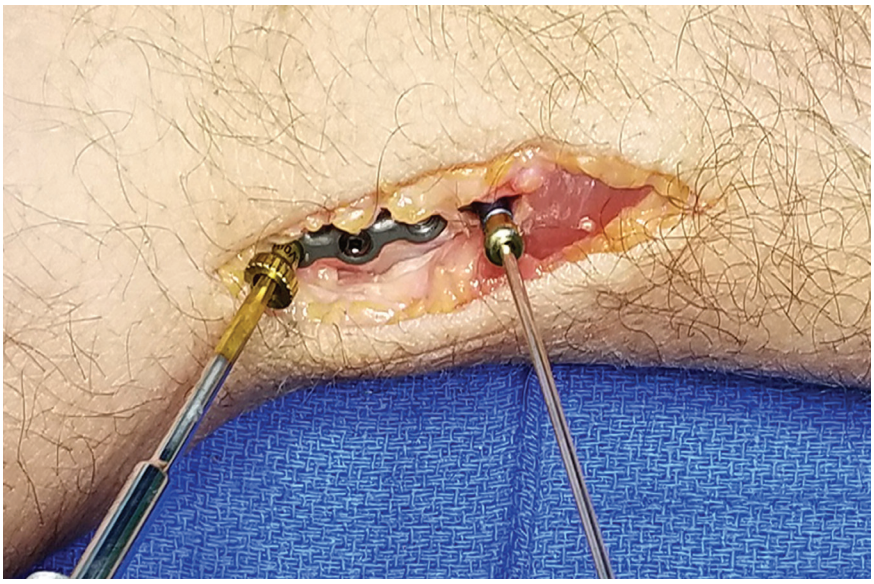


14 PLS K-WIRE INSERTION

Insert the gold end of the .9mm K-wire through the PLS A.I.M.ing Guide in the desired trajectory until the far cortex is reached.

Confirm that the desired trajectory has been achieved using fluoroscopy.

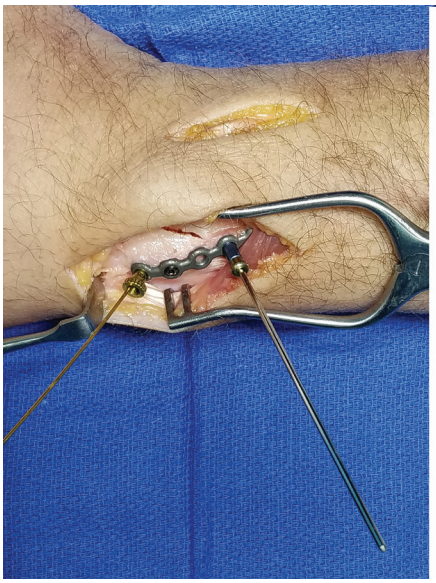


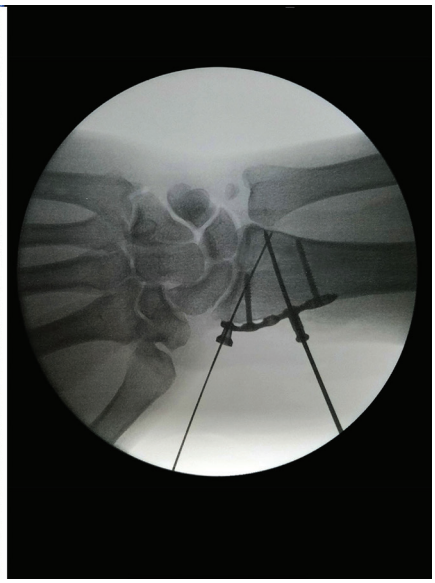


15 PLS A.I.M.ing GUIDE REMOVAL

Slide the PLS Initial Driver over the K-wire to engage and remove the PLS A.I.M.ing Guide.

Note: Be sure to leave the .9mm K-wire in place.

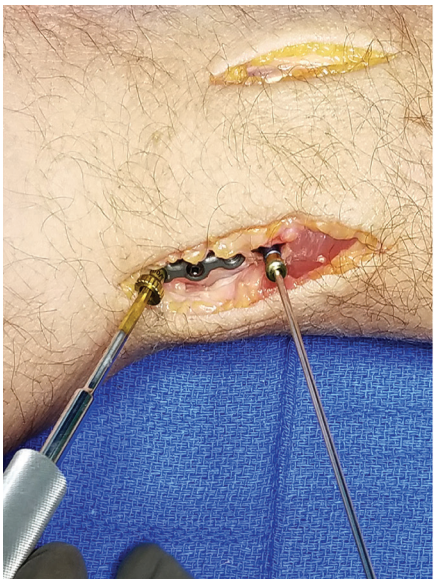


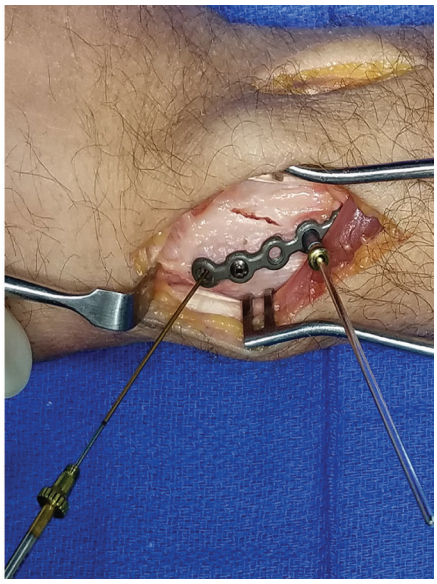


16 PLS SCREW PREPARATION

Slide the cannulated PLS Depth Gauge over the K-wire until flush against the plate and measure the screw length.

Remove the depth gauge leaving the K-wire in place. Then drill over the K-wire using the 2.0mm Cannulated Drill up to the far cortex.

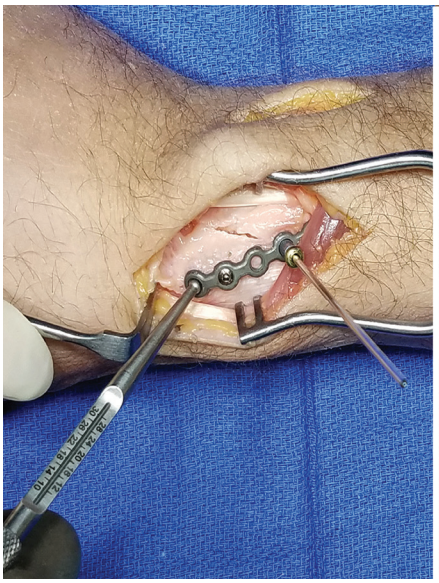


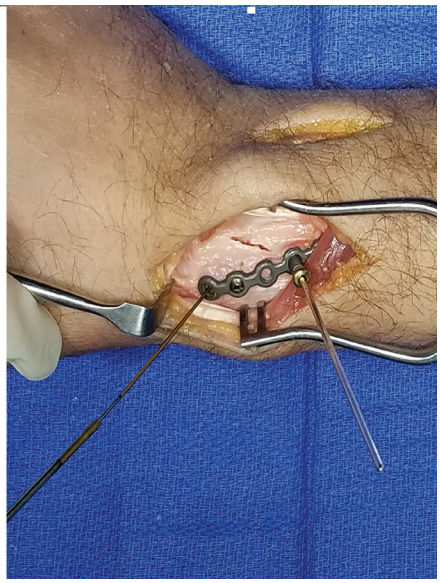

17 PLS SCREW INSERTION

Using the PLS Initial Driver, insert the PLS over the K-wire and into the desired trajectory until the head of the PLS engages the plate.

Remove the K-wire and the PLS Initial Driver.

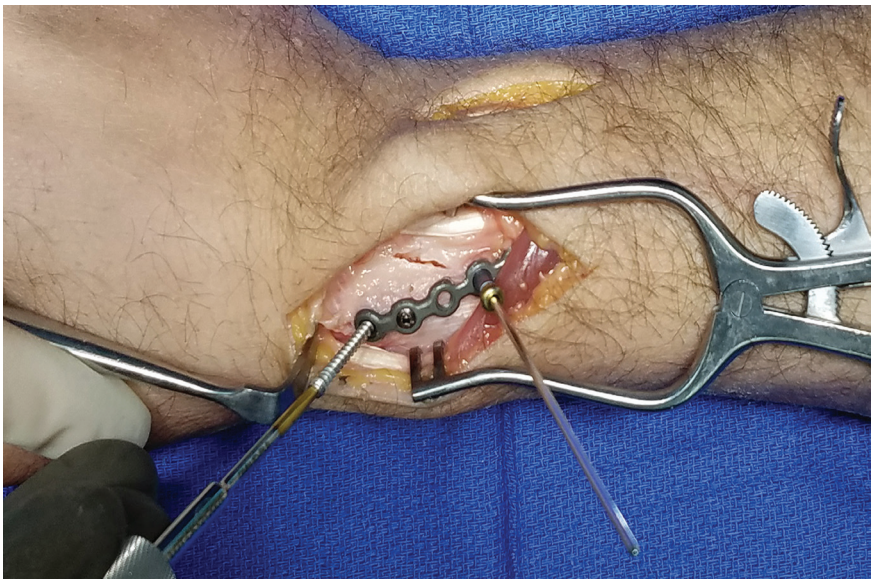


18 USING THE PLS INITIAL DRIVER, INSERT THE PLS


Securely hold the respective node using the Bending Pliers.

Use the stronger PLS Final Driver to fully engage the screw.



Final Driver, PLS

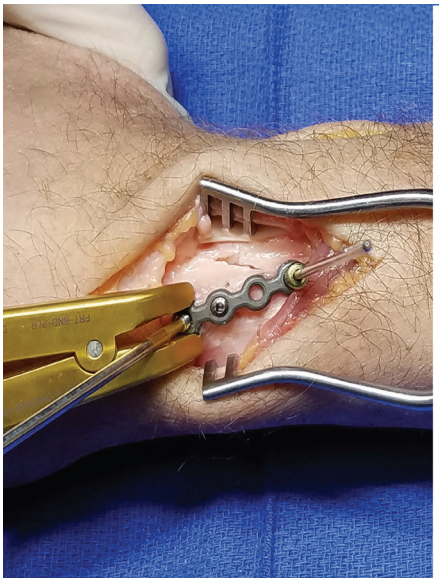

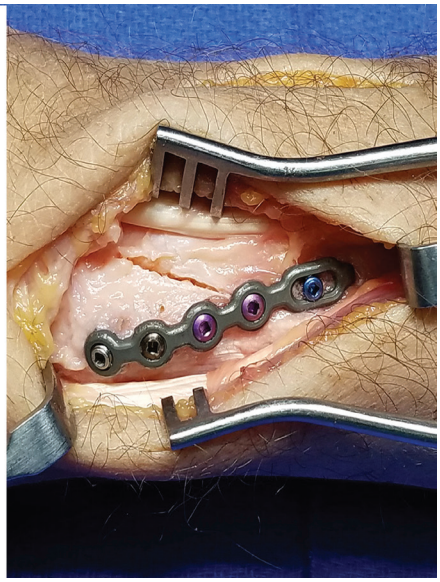


19 FLUOROSCOPIC CONFIRMATION


Confirm the reduction, proper screw placement and screw length using fluoroscopy.

Confirm that all screws have been fully tightened.

Repair soft tissues as needed, then close the incision in your normal fashion.

Note: Confirm that all PDG's have been removed even if the respective node has not been used.

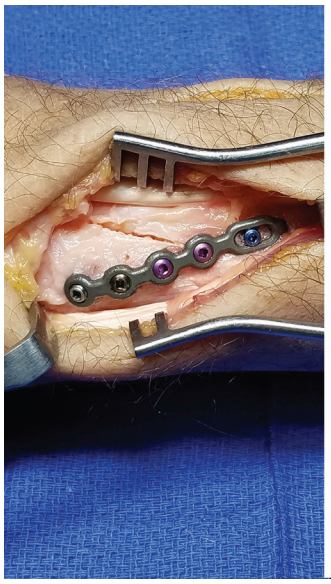

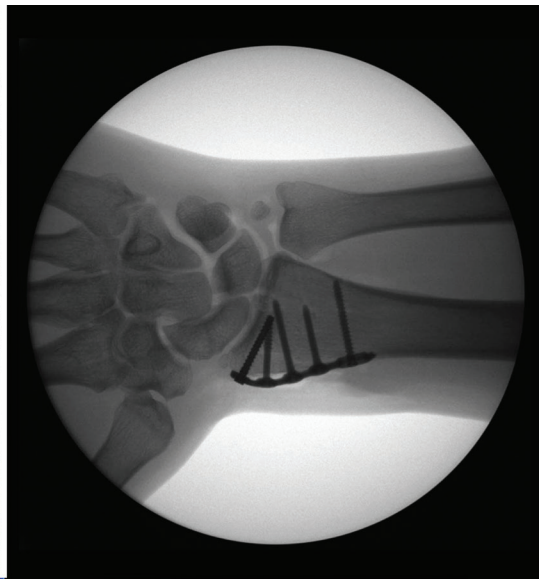


01 FRACTURE REDUCTION

Apply traction to reduce the fracture.

Achieving adequate reduction may require additional manipulation.

Confirm fracture reduction using fluoroscopy.

Note: Finger trap traction may be helpful in maintaining the reduction.

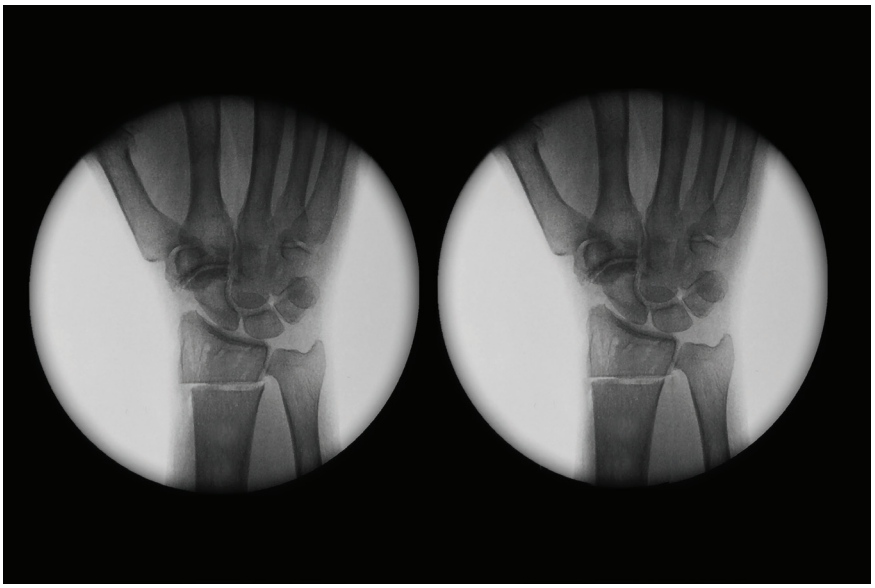


02 ATTACHING INSERTION HANDLE

The Dorsal Spanning Plates are offered in two lengths: short and long. They are also anatomically designed with a metacarpal and radial end.

Select the appropriate length Dorsal Spanning Plate and attach the Insertion Handle to the most proximal hole at the metacarpal end.

Using the T-10 driver, confirm that the Insertion Handle locking screw is fully tightened.



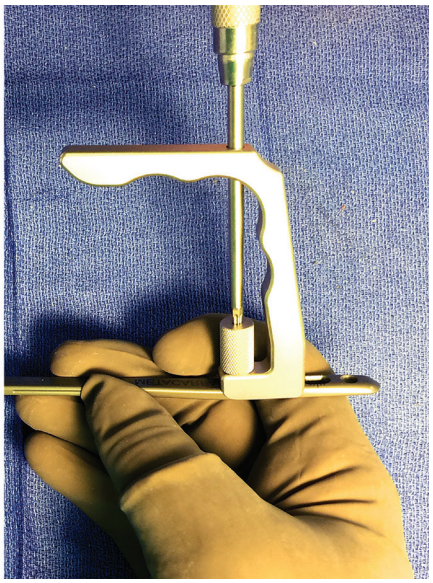




03 PLATE POSITIONING

Correctly orient the plate on the skin over the 2nd or 3rd metacarpal and the radius.

Verify the plate positioning using fluoroscopy, then mark the distal and proximal end points.



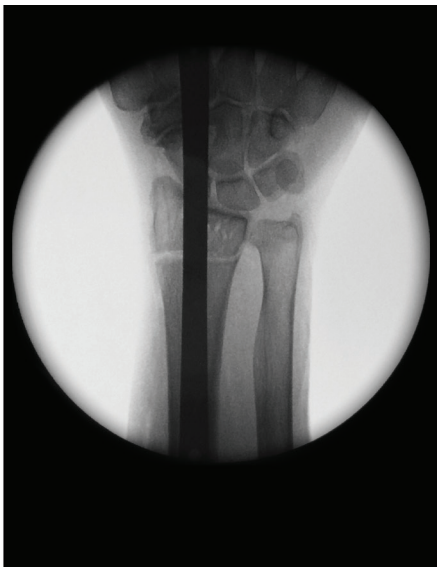




04 DISTAL EXPOSURE

Make a 3cm incision centered over the metacarpal.

Notes: If placed on the 2nd metacarpal, ensure that the plate is inserted under the EPL and through the 2nd extensor compartment.

If placed on the 3rd metacarpal, release and mobilize the third and fourth compartments to allow the plate to pass beneath the tendons.

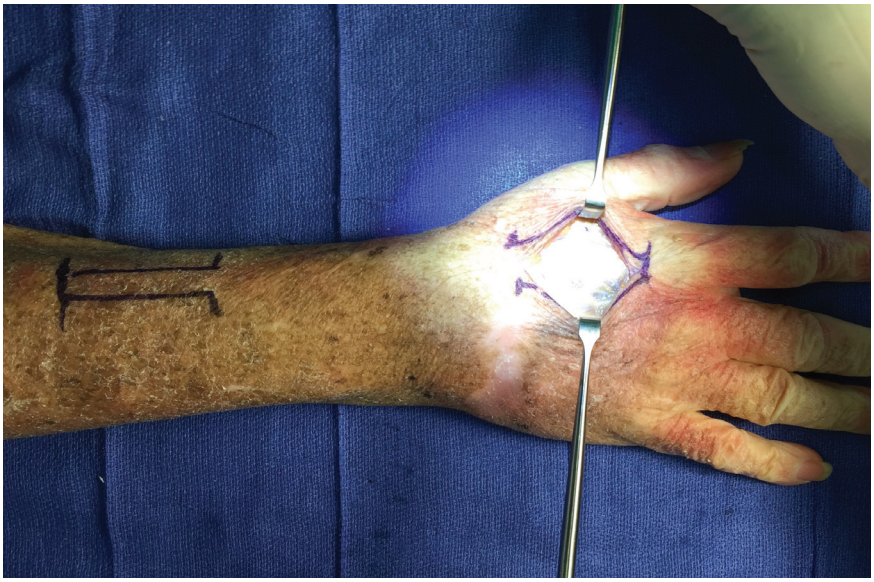



05 PLATE INSERTION

Insert the plate retrograde through the distal incision along the dorsal surface of the radius.

Verify the extensor tendons remain superficial to the plate.

Verify the plate positioning and confirm fracture reduction using fluoroscopy.

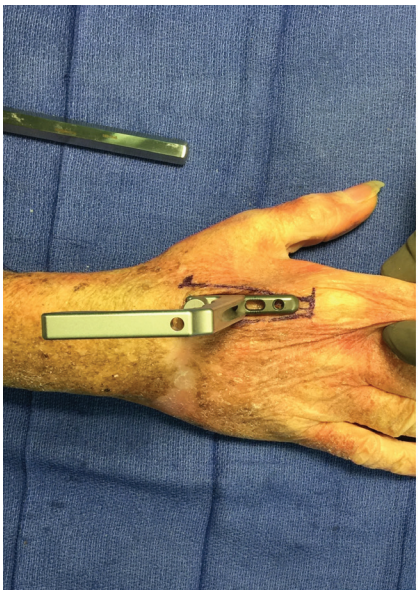

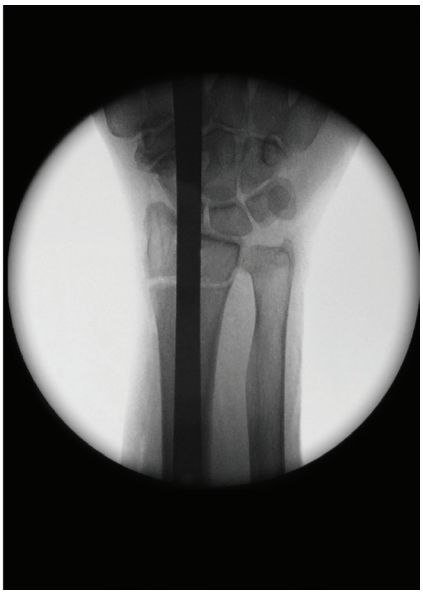

06 PROXIMAL EXPOSURE

Make a 4cm incision at the level of the previously marked location to expose the radial shaft.

Be sure to identify and protect the radial sensory nerve.




07 PROVISIONAL DISTAL FIXATION


Drill through the gliding hole on the metacarpal end of the plate using the 2.3mm bit.

Measure the screw length directly through the plate using the Depth Gauge taking note of the scale with the symbol: .

Insert and fully tighten a 3.0mm Compression Screw using the T-10 driver.



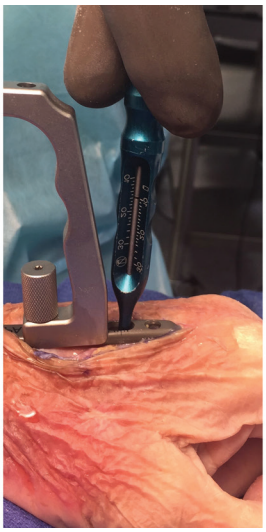

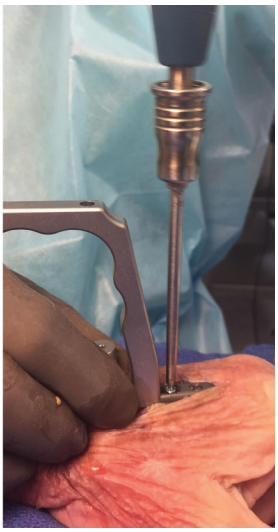




Compression Screw



Drill, 2.3mm




Depth Gauge, Standard

08 FLUOROSCOPIC CONFIRMATION

Confirm proper screw placement and length using fluoroscopy.


Caution: Prevent excessive screw length as this can potentially cause soft tissue irritation.




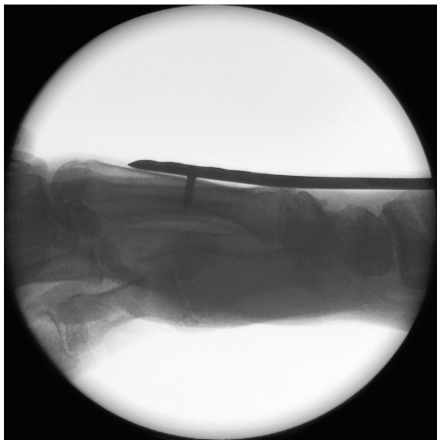

09 INSERTION HANDLE REMOVAL

Using the T-10 driver, loosen the Lock Screw and remove the Insertion Handle.

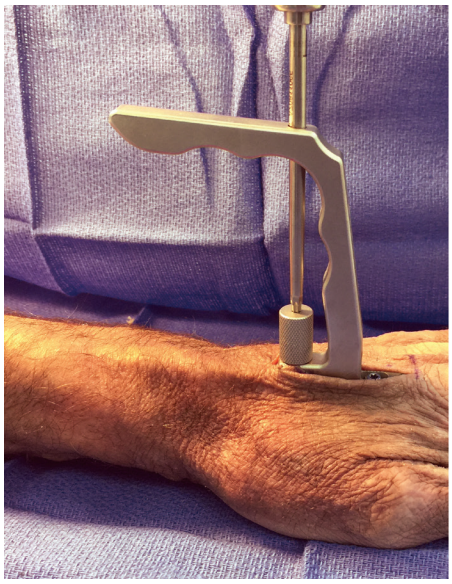


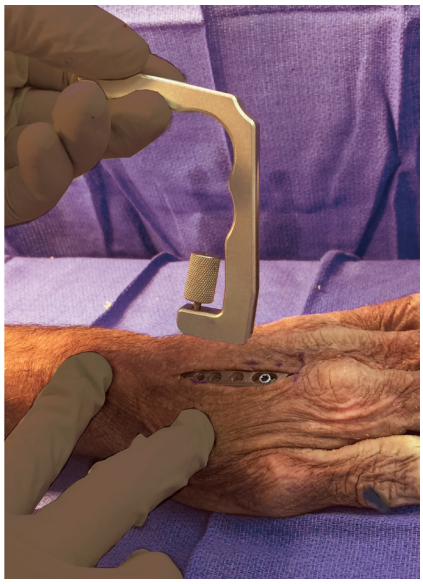


10 FRACTURE REDUCTION

Adjust traction as needed to achieve fracture reduction.

Confirm that radial length and a proper reduction have been achieved using fluoroscopy.

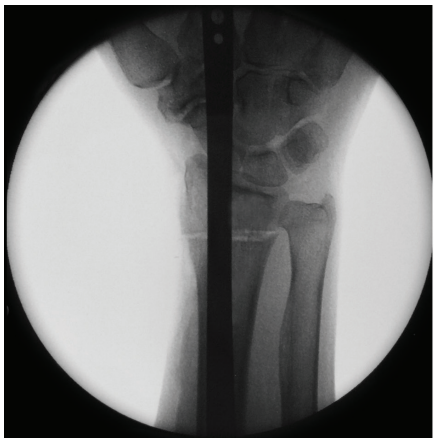


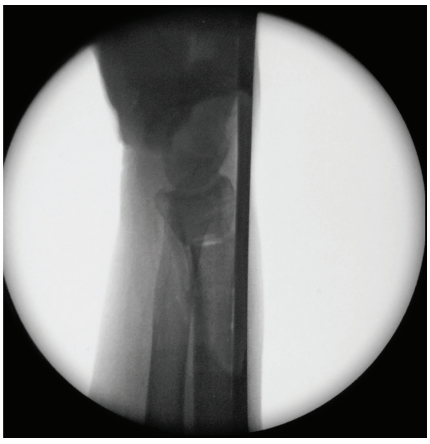

11 PROVISIONAL PROXIMAL FIXATION

Drill, measure and insert a 3.0mm Compression Screw into the gliding hole on the radial end of the plate.

Confirm proper screw placement and length using fluoroscopy.

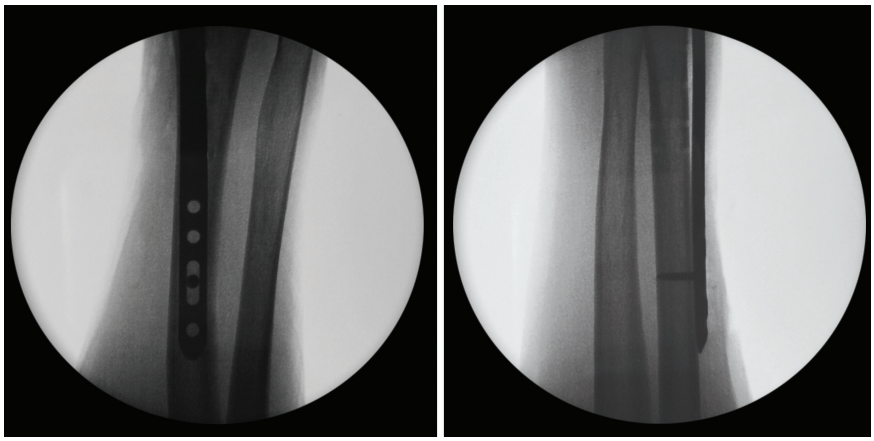


12 FINAL PLATE FIXATION

Secure the 2.3mm Thread-In Drill Guide into a threaded hole of the plate.

Drill through the Thread-In Drill Guide, then measure the screw length using the etched marks on the side of the bit.

Remove the Thread-In Drill Guide, then insert and fully tighten either a 3.0mm Compression or Locking Screw using the T-10 driver.

Repeat this step for the remaining holes at both ends of the plate.

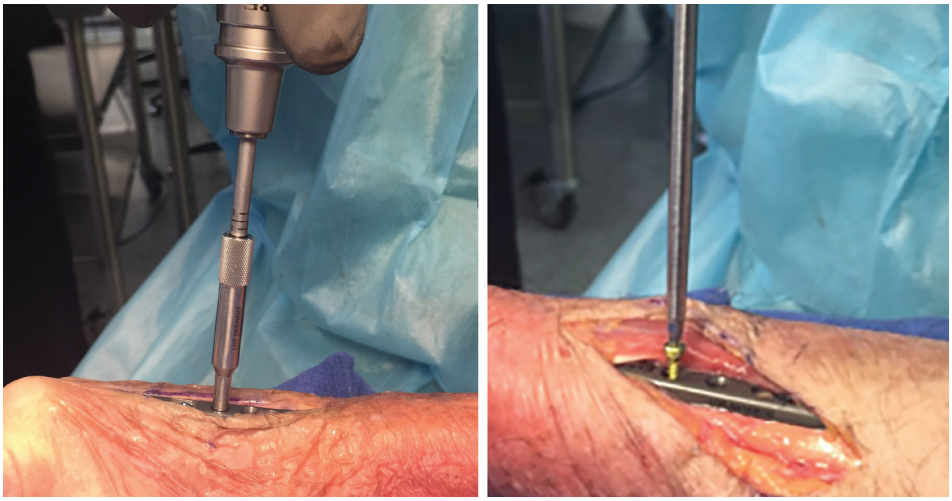



Thread-in Drill Guide, 2.3mm



Screw, Multi-Thread, Locking, 3.0mm

13 FINAL CONFIRMATION & WOUND CLOSURE

Confirm proper reduction, screw length and placement using fluoroscopy.

Close the incisions in your normal fashion.

After the fracture has healed, the plate is removed through the distal incision.



01 PLATE SETUP

The GEMINUS system includes a pair of Plate Benders used to manipulate each head of the GEMINUS plate independently.

The Plate Holder is designed to secure the shaft of the GEMINUS plate during manipulation. The plate holder has openings at each end that are size specific to the length of the plate's shaft.

The plate bender has three slots to manipulate the head of each plate size and configuration (with or without PDG's).

Note: The head should fit snug within the selected slot.




02 ADJUSTING VOLAR TILT


With the shaft of the plate secured into the Plate Holder, use the Plate Bender to manipulate the plate to achieve the desired angle.

Note: When bending the plate, make small adjustments until the desired angle is achieved.

Warning: Bending may weaken or break the plate. Be sure to inspect the plate for damage prior to use.

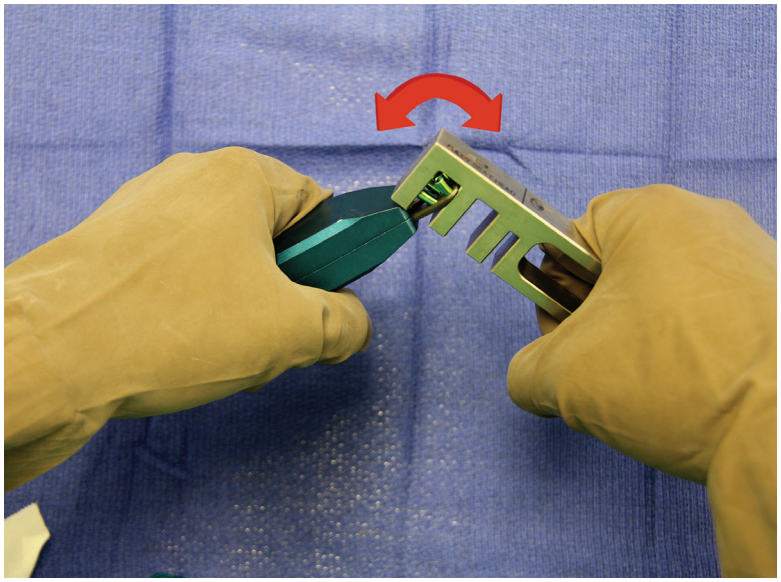

GEMINUS® Volar Distal Radius Plating System - Cat.# GMN-FSP-SYS

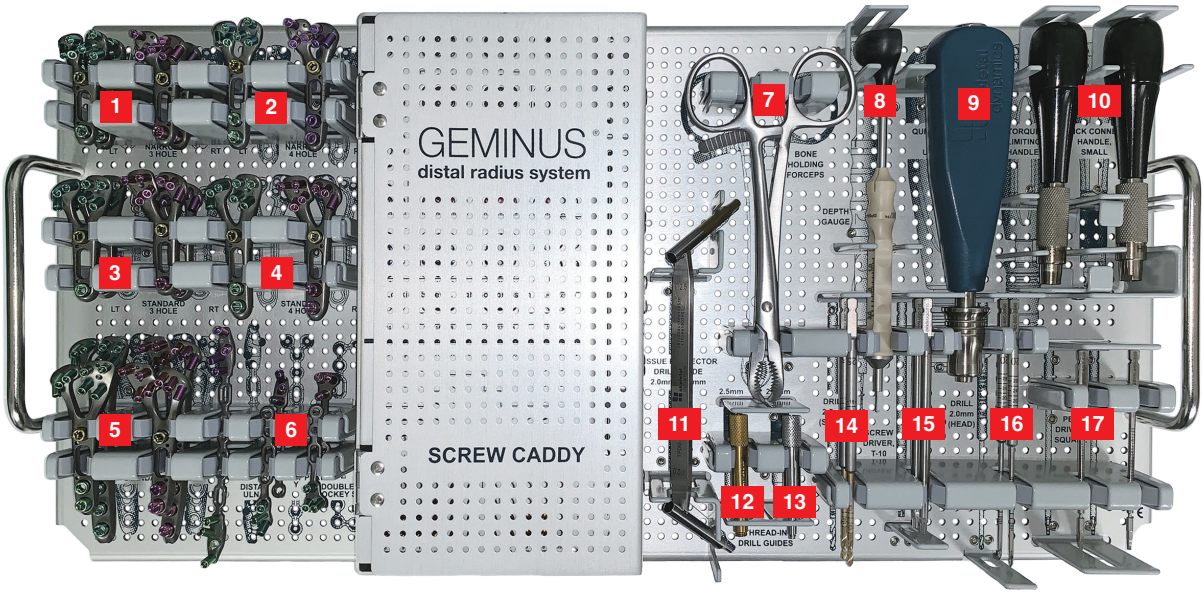


Loc #	Catalog #	Description
1	GMN-LTS-4HL	GEMINUS Plate, Standard, 4 Hole, Left
	GMN-RTS-4HL	GEMINUS Plate, Standard, 4 Hole, Right
2	GMN-LTS-3HL	GEMINUS Plate, Standard, 3 Hole, Left
	GMN-RTS-3HL	GEMINUS Plate, Standard, 3 Hole, Right
3	GMN-LTN-3HL	GEMINUS Plate, Narrow, 3 Hole, Left
	GMN-RTN-3HL	GEMINUS Plate, Narrow, 3 Hole, Right
	GMN-LTN-4HL	GEMINUS Plate, Narrow, 4 Hole, Left
	GMN-RTN-4HL	GEMINUS Plate, Narrow, 4 Hole, Right
4	GMN-LTW-4HL	GEMINUS Plate, Wide, 4 Hole, Left
	GMN-RTW-4HL	GEMINUS Plate, Wide, 4 Hole, Right
5	GMN-LTS-7HL	GEMINUS Plate, Standard, 7 Hole, Left
	GMN-RTS-7HL	GEMINUS Plate, Standard, 7 Hole, Right
6	PRT-FSP-DU	PROTEAN Fragment Plate, Distal Ulna
	PRT-RCP-RT	PROTEAN Fragment Plate, Radial Column Plate, Right
	PRT-RCP-LT	PROTEAN Fragment Plate, Radial Column Plate, Left
	PRT-CCP-RT	PROTEAN Fragment Plate, Central Column Plate, Right
	PRT-CCP-LT	PROTEAN Fragment Plate, Central Column Plate, Left
	PRT-FSP-YS	PROTEAN Fragment Plate, Y - Straight*
	PRT-FSP-LR	PROTEAN Fragment Plate, Double Hockey Stick*
7	FRCP-BHM-RTC	Forceps, Bone Holding
8	DPGA-UNV-030	Depth Gauge, Universal, 30mm
9	HNDL-UQC-FXD	Handle, Universal Quick Connect
10	HNDL-SQC-FXD	Handle, Small Quick Connect
11	TPDG-DSD-2025	Tissue Protector / Drill Guide, 2.0mm x 2.5mm
12	TPDG-THD-DG25	Thread-in Drill Guide, 2.5mm
13	TPDG-THD-DG20	Thread-in Drill Guide, 2.0mm
14	DRLL-SSC-25040	Drill, 2.5mm x 40mm
15	DRVR-UQC-T10	Driver, T10
16	DRLL-SSC-20040	Drill, 2.0mm x 40mm
17	DRVR-AOS-S20	Driver, Square Tip 2.0mm


**Available upon request only.*

GEMINUS VOLAR PLATES


NARROW: 3 & 4 Hole

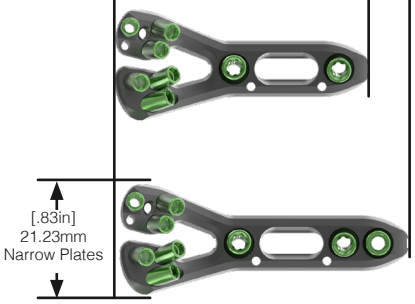


STANDARD: 3, 4 & 7 Hole

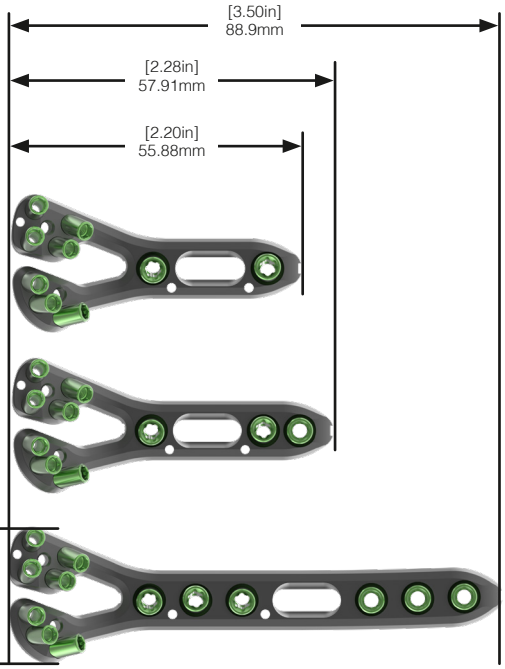

WIDE: 4 Hole

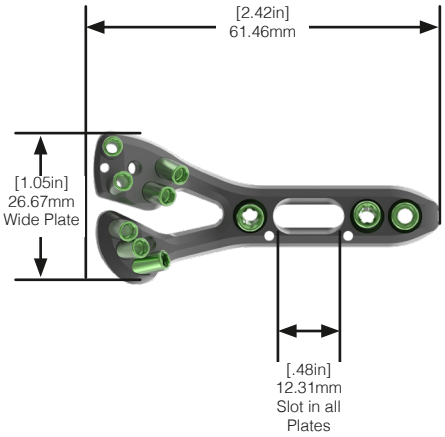


XL: 120mm, 160mm, 200mm

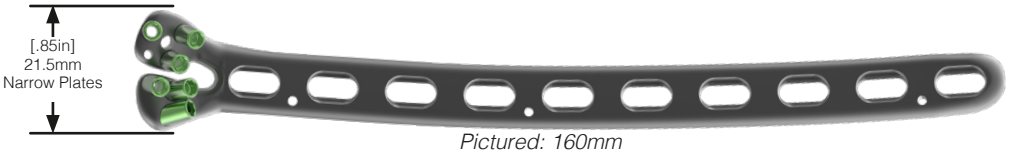


Pictured: 160mm

PROTEAN FRAGMENT PLATES


PROTEAN Fragment Plate, Y - Straight

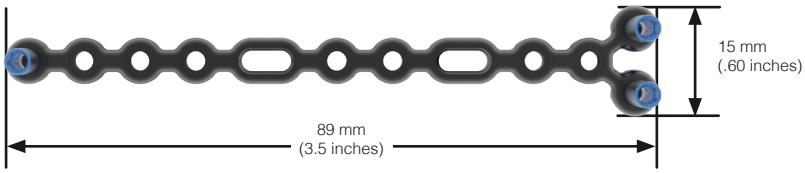


PROTEAN Fragment Plate, Central Column

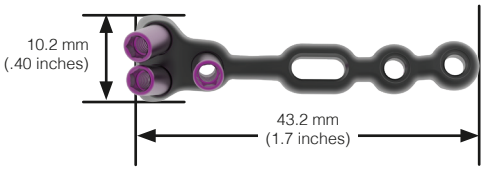


PROTEAN Fragment Plate, Double Hockey Stick

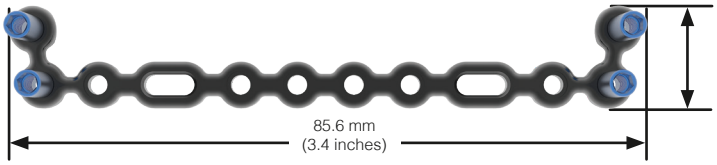


PROTEAN Fragment Plate, Radial Column

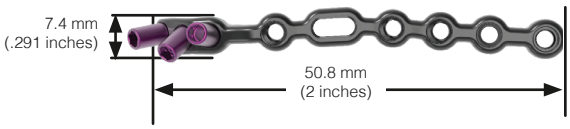

PROTEAN Fragment Plate, Distal Ulna

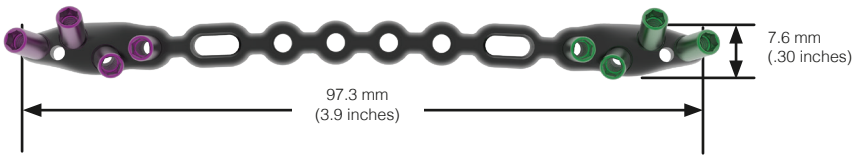


PROTEAN FRAGMENT PLATES (Cont.)

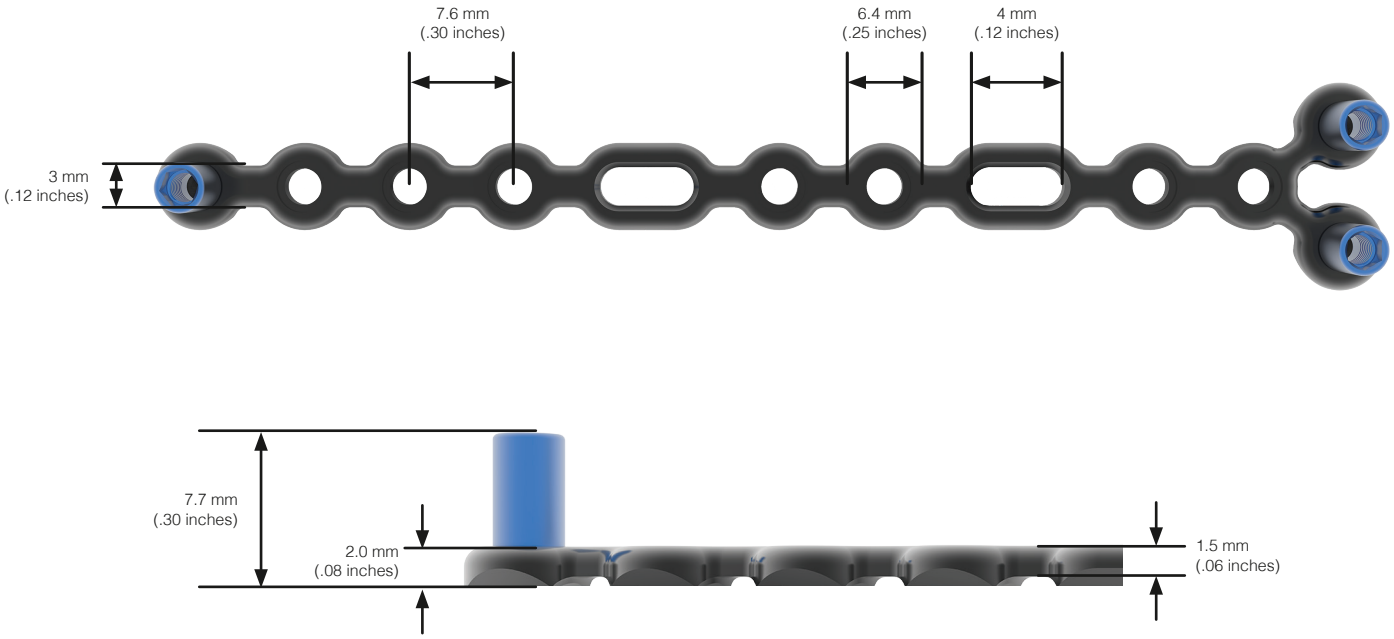

SINGLE USE INSTRUMENTS

	Catalog #	Description
	DRLL-SSC-20040	Drill, 2.0mm x 40mm
	DRLL-SSC-25040	Drill, 2.5mm x 40mm
	DRLL-PLS-20	Drill, Cannulated 2.0mm x 40mm
	DRVR-AOS-S20	Driver, Square Tip 2.0mm
	DRVR-UQC-T10	Driver, Quick Connect T10
	DRVR-AOS-PLS	Final Driver, PLS
	PDG-AIM-015	A.I.M.ing Guide, 1.6mm
	KWIR-STD-09152	K-Wire, .9mm x 152mm
	KWIR-STD-15127	K-Wire, 1.6mm x 127mm
	PLS-AIM-0910	PLS A.I.M.ing Guide

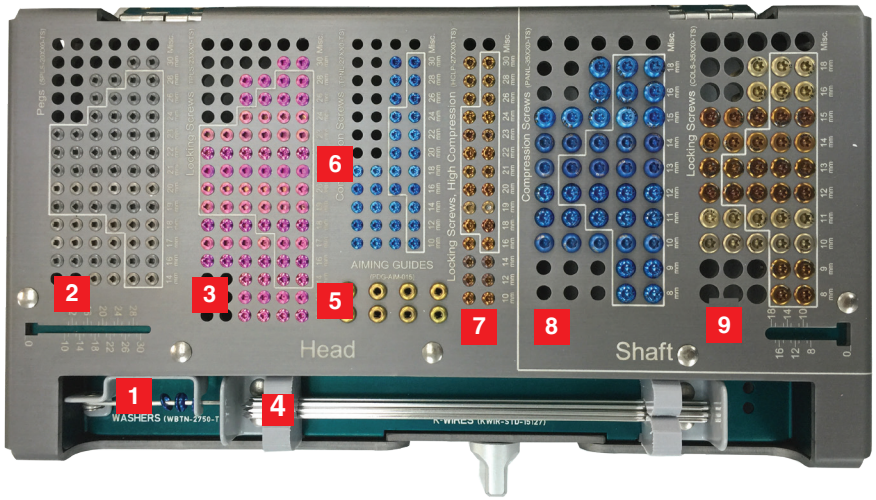


Loc #	Catalog #	Description
1	WBTN-2750-T	Washer, Button, Inside Ø2.7mm, Outside Ø5.0mm, Ti
2	SPLS-20100-TS	Smooth Peg, Locking, 2.0mm x 10mm, Ti
	SPLS-20120-TS	Smooth Peg, Locking, 2.0mm x 12mm, Ti
	SPLS-20140-TS	Smooth Peg, Locking, 2.0mm x 14mm, Ti
	SPLS-20160-TS	Smooth Peg, Locking, 2.0mm x 16mm, Ti
	SPLS-20170-TS	Smooth Peg, Locking, 2.0mm x 17mm, Ti
	SPLS-20180-TS	Smooth Peg, Locking, 2.0mm x 18mm, Ti
	SPLS-20190-TS	Smooth Peg, Locking, 2.0mm x 19mm, Ti
	SPLS-20200-TS	Smooth Peg, Locking, 2.0mm x 20mm, Ti
	SPLS-20210-TS	Smooth Peg, Locking, 2.0mm x 21mm, Ti
	SPLS-20220-TS	Smooth Peg, Locking, 2.0mm x 22mm, Ti
	SPLS-20230-TS	Smooth Peg, Locking, 2.0mm x 23mm, Ti
	SPLS-20240-TS	Smooth Peg, Locking, 2.0mm x 24mm, Ti
	SPLS-20260-TS	Smooth Peg, Locking, 2.0mm x 26mm, Ti
	SPLS-20280-TS	Smooth Peg, Locking, 2.0mm x 28mm, Ti
	SPLS-20300-TS	Smooth Peg, Locking, 2.0mm x 30mm, Ti
3	TPLS-23100-TS	Threaded Peg, Locking, 2.3mm x 10mm, Ti
	TPLS-23120-TS	Threaded Peg, Locking, 2.3mm x 12mm, Ti
	TPLS-23140-TS	Threaded Peg, Locking, 2.3mm x 14mm, Ti
	TPLS-23160-TS	Threaded Peg, Locking, 2.3mm x 16mm, Ti
	TPLS-23170-TS	Threaded Peg, Locking, 2.3mm x 17mm, Ti
	TPLS-23180-TS	Threaded Peg, Locking, 2.3mm x 18mm, Ti
	TPLS-23190-TS	Threaded Peg, Locking, 2.3mm x 19mm, Ti
	TPLS-23200-TS	Threaded Peg, Locking, 2.3mm x 20mm, Ti
	TPLS-23210-TS	Threaded Peg, Locking, 2.3mm x 21mm, Ti
	TPLS-23220-TS	Threaded Peg, Locking, 2.3mm x 22mm, Ti
	TPLS-23230-TS	Threaded Peg, Locking, 2.3mm x 23mm, Ti
	TPLS-23240-TS	Threaded Peg, Locking, 2.3mm x 24mm, Ti
	TPLS-23260-TS	Threaded Peg, Locking, 2.3mm x 26mm, Ti
	TPLS-23280-TS	Threaded Peg, Locking, 2.3mm x 28mm, Ti
	TPLS-23300-TS	Threaded Peg, Locking, 2.3mm x 30mm, Ti
4	KWIR-STD-15127	K-Wire, Standard Tip, 1.6mm x 127mm

SCREW CADDY (Cont.)

Loc #		Catalog #	Description
5		PDG-AIM-015	A.I.M.ing Guides, 1.6mm
6		TPNL-27100-TS	Threaded Peg, Non Locking, 2.7mm x 10mm, Ti
		TPNL-27120-TS	Threaded Peg, Non Locking, 2.7mm x 12mm, Ti
		TPNL-27140-TS	Threaded Peg, Non Locking, 2.7mm x 14mm, Ti
		TPNL-27160-TS	Threaded Peg, Non Locking, 2.7mm x 16mm, Ti
		TPNL-27180-TS	Threaded Peg, Non Locking, 2.7mm x 18mm, Ti
		TPNL-27200-TS	Threaded Peg, Non Locking, 2.7mm x 20mm, Ti
		TPNL-27220-TS	Threaded Peg, Non Locking, 2.7mm x 22mm, Ti
		TPNL-27240-TS	Threaded Peg, Non Locking, 2.7mm x 24mm, Ti
		TPNL-27260-TS	Threaded Peg, Non Locking, 2.7mm x 26mm, Ti
		TPNL-27280-TS	Threaded Peg, Non Locking, 2.7mm x 28mm, Ti
		TPNL-27300-TS	Threaded Peg, Non Locking, 2.7mm x 30mm, Ti
7		HCLP-27100-TS	High Compression Locking Peg, 2.7mm x 10mm, Ti
		HCLP-27120-TS	High Compression Locking Peg, 2.7mm x 12mm, Ti
		HCLP-27140-TS	High Compression Locking Peg, 2.7mm x 14mm, Ti
		HCLP-27160-TS	High Compression Locking Peg, 2.7mm x 16mm, Ti
		HCLP-27180-TS	High Compression Locking Peg, 2.7mm x 18mm, Ti
		HCLP-27190-TS	High Compression Locking Peg, 2.7mm x 19mm, Ti
		HCLP-27200-TS	High Compression Locking Peg, 2.7mm x 20mm, Ti
		HCLP-27210-TS	High Compression Locking Peg, 2.7mm x 21mm, Ti
		HCLP-27220-TS	High Compression Locking Peg, 2.7mm x 22mm, Ti
		HCLP-27230-TS	High Compression Locking Peg, 2.7mm x 23mm, Ti
		HCLP-27240-TS	High Compression Locking Peg, 2.7mm x 24mm, Ti
		HCLP-27260-TS	High Compression Locking Peg, 2.7mm x 26mm, Ti
		HCLP-27280-TS	High Compression Locking Peg, 2.7mm x 28mm, Ti
		HCLP-27300-TS	High Compression Locking Peg, 2.7mm x 30mm, Ti
8		PANL-35080-TS	Screw, Cortical Non Locking, 3.5mm x 8mm, Ti
		PANL-35090-TS	Screw, Cortical Non Locking, 3.5mm x 9mm, Ti
		PANL-35100-TS	Screw, Cortical Non Locking, 3.5mm x 10mm, Ti
		PANL-35110-TS	Screw, Cortical Non Locking, 3.5mm x 11mm, Ti
		PANL-35120-TS	Screw, Cortical Non Locking, 3.5mm x 12mm, Ti
		PANL-35130-TS	Screw, Cortical Non Locking, 3.5mm x 13mm, Ti
		PANL-35140-TS	Screw, Cortical Non Locking, 3.5mm x 14mm, Ti
		PANL-35150-TS	Screw, Cortical Non Locking, 3.5mm x 15mm, Ti
		PANL-35160-TS	Screw, Cortical Non Locking, 3.5mm x 16mm, Ti
		PANL-35180-TS	Screw, Cortical Non Locking, 3.5mm x 18mm, Ti
9		COLS-35080-TS	Screw, Cortical Locking, 3.5mm x 8mm, Ti
		COLS-35090-TS	Screw, Cortical Locking, 3.5mm x 9mm, Ti
		COLS-35100-TS	Screw, Cortical Locking, 3.5mm x 10mm, Ti
		COLS-35110-TS	Screw, Cortical Locking, 3.5mm x 11mm, Ti
		COLS-35120-TS	Screw, Cortical Locking, 3.5mm x 12mm, Ti
		COLS-35130-TS	Screw, Cortical Locking, 3.5mm x 13mm, Ti
		COLS-35140-TS	Screw, Cortical Locking, 3.5mm x 14mm, Ti

PLS and HPE MODULE (Bottom Base of Tray)

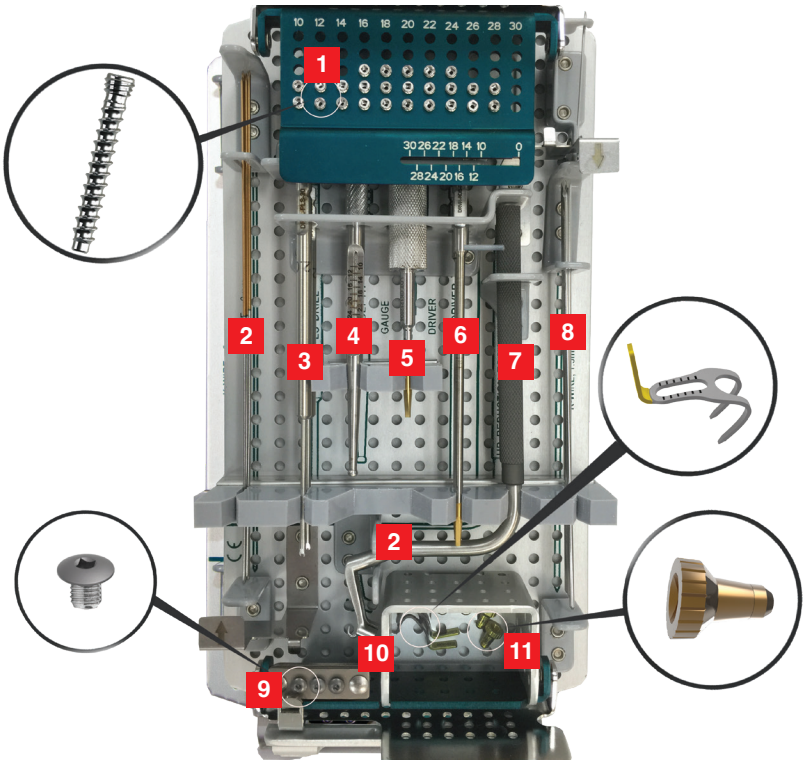


Loc #	Catalog #	Description
1	PALS-25100-CC	Screw, Polyaxial Locking, 2.5mm x 10mm Cannulated, CoCr
	PALS-25120-CC	Screw, Polyaxial Locking, 2.5mm x 12mm Cannulated, CoCr
	PALS-25140-CC	Screw, Polyaxial Locking, 2.5mm x 14mm Cannulated, CoCr
	PALS-25160-CC	Screw, Polyaxial Locking, 2.5mm x 16mm Cannulated, CoCr
	PALS-25180-CC	Screw, Polyaxial Locking, 2.5mm x 18mm Cannulated, CoCr
	PALS-25200-CC	Screw, Polyaxial Locking, 2.5mm x 20mm Cannulated, CoCr
	PALS-25220-CC	Screw, Polyaxial Locking, 2.5mm x 22mm Cannulated, CoCr
	PALS-25240-CC	Screw, Polyaxial Locking, 2.5mm x 24mm Cannulated, CoCr
	PALS-25260-CC	Screw, Polyaxial Locking, 2.5mm x 26mm Cannulated, CoCr
	PALS-25280-CC	Screw, Polyaxial Locking, 2.5mm x 28mm Cannulated, CoCr
	PALS-25300-CC	Screw, Polyaxial Locking, 2.5mm x 30mm Cannulated, CoCr
2	KWIR-STD-09152	K-Wire, Standard Tip, .9mm x 152mm
3	DRLL-PLS-20	Drill, Cannulated, Polyaxial Locking Screw, 2.0mm
4	GMN-CDG-PLS	Cannulated Depth Gauge, Polyaxial Locking Screw
5	GMN-ID-PLS	Initial Driver, Polyaxial Locking Screw
6	DRVR-AOS-PLS	Driver, AO Connection, Polyaxial Locking Screw
7	GMN-HP-DG15	GEMINUS Hook Plate Reduction Tool
8	KWIR-STD-15127	K-Wire, Standard Tip, 1.6mm x 127mm
9	GMN-HP-SCRW	GEMINUS Hook Plate, Screw
10	GMN-HP	GEMINUS Hook Plate
11	PLS-AIM-0910	PLS A.I.M.ing Guide

ACCESSORY INSTRUMENTATION (Bottom Base of Tray)


Loc #	Catalog #	Description
12	GMN-FSP-PLB	GEMINUS Plate Bender
13	GMN-FSP-PLH	GEMINUS Plate Holder
14	PRT-BND-PLR	PROTEAN Bending Pliers



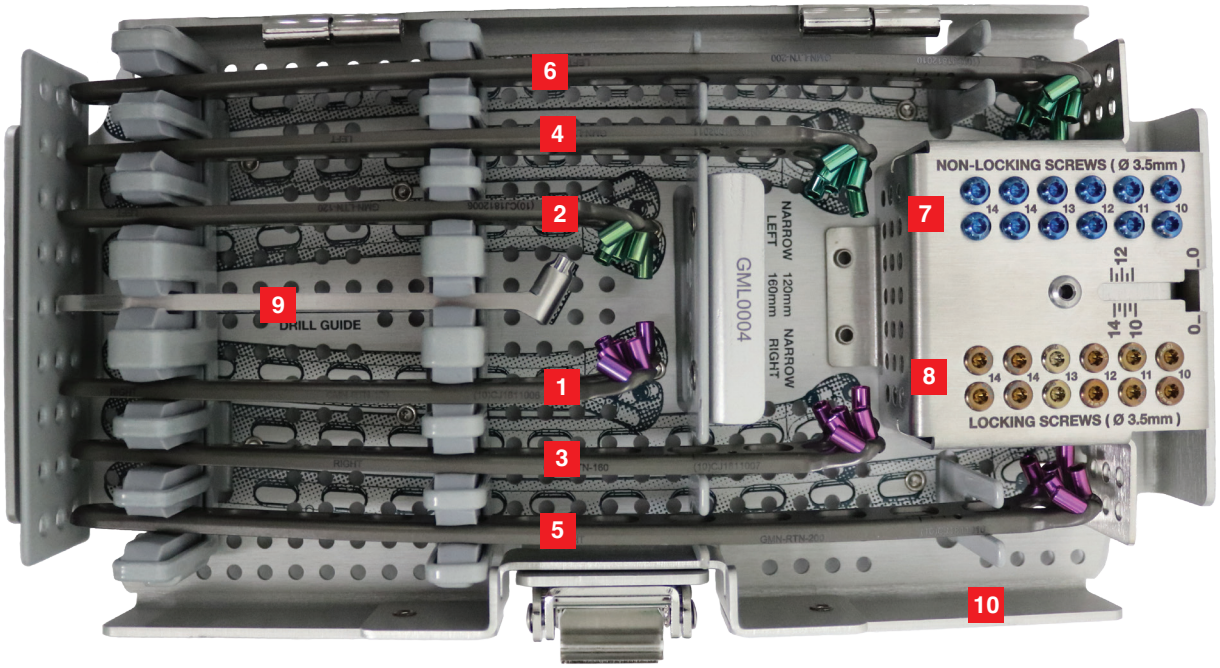

Loc #	Catalog #	Description
1	GMN-RTN-120	Assembled, GEMINUS VDR Plate, Narrow, 120mm, Right
2	GMN-LTN-120	Assembled, GEMINUS VDR Plate, Narrow, 120mm, Left
3	GMN-RTN-160	Assembled, GEMINUS VDR Plate, Narrow, 160mm, Right
4	GMN-LTN-160	Assembled, GEMINUS VDR Plate, Narrow, 160mm, Left
5	GMN-RTN-200	Assembled, GEMINUS VDR Plate, Narrow, 200mm, Right
6	GMN-LTN-200	Assembled, GEMINUS VDR Plate, Narrow, 200mm, Left
7	PANL-35080-TS	Screw, Cortical Non Locking, 3.5mm x 8mm, Ti
	PANL-35090-TS	Screw, Cortical Non Locking, 3.5mm x 9mm, Ti
	PANL-35100-TS	Screw, Cortical Non Locking, 3.5mm x 10mm, Ti
	PANL-35110-TS	Screw, Cortical Non Locking, 3.5mm x 11mm, Ti
	PANL-35120-TS	Screw, Cortical Non Locking, 3.5mm x 12mm, Ti
	PANL-35130-TS	Screw, Cortical Non Locking, 3.5mm x 13mm, Ti
	PANL-35140-TS	Screw, Cortical Non Locking, 3.5mm x 14mm, Ti
	PANL-35150-TS	Screw, Cortical Non Locking, 3.5mm x 15mm, Ti
	PANL-35160-TS	Screw, Cortical Non Locking, 3.5mm x 16mm, Ti
	PANL-35180-TS	Screw, Cortical Non Locking, 3.5mm x 18mm, Ti
8	COLS-35080-TS	Screw, Cortical Locking, 3.5mm x 8mm, Ti
	COLS-35090-TS	Screw, Cortical Locking, 3.5mm x 9mm, Ti
	COLS-35100-TS	Screw, Cortical Locking, 3.5mm x 10mm, Ti
	COLS-35110-TS	Screw, Cortical Locking, 3.5mm x 11mm, Ti
	COLS-35120-TS	Screw, Cortical Locking, 3.5mm x 12mm, Ti
	COLS-35130-TS	Screw, Cortical Locking, 3.5mm x 13mm, Ti
	COLS-35140-TS	Screw, Cortical Locking, 3.5mm x 14mm, Ti
	COLS-35150-TS	Screw, Cortical Locking, 3.5mm x 15mm, Ti
	COLS-35160-TS	Screw, Cortical Locking, 3.5mm x 16mm, Ti
	COLS-35180-TS	Screw, Cortical Locking, 3.5mm x 18mm, Ti
9	TPDG-GTS-25	Tissue Protector/Drill Guide, Slot, 2.5mm
10	GMN-LNG-MOD	GEMINUS XL Volar Distal Radius Plate Module

DORSAL SPANNIG PLATE SET CONFIGURATION

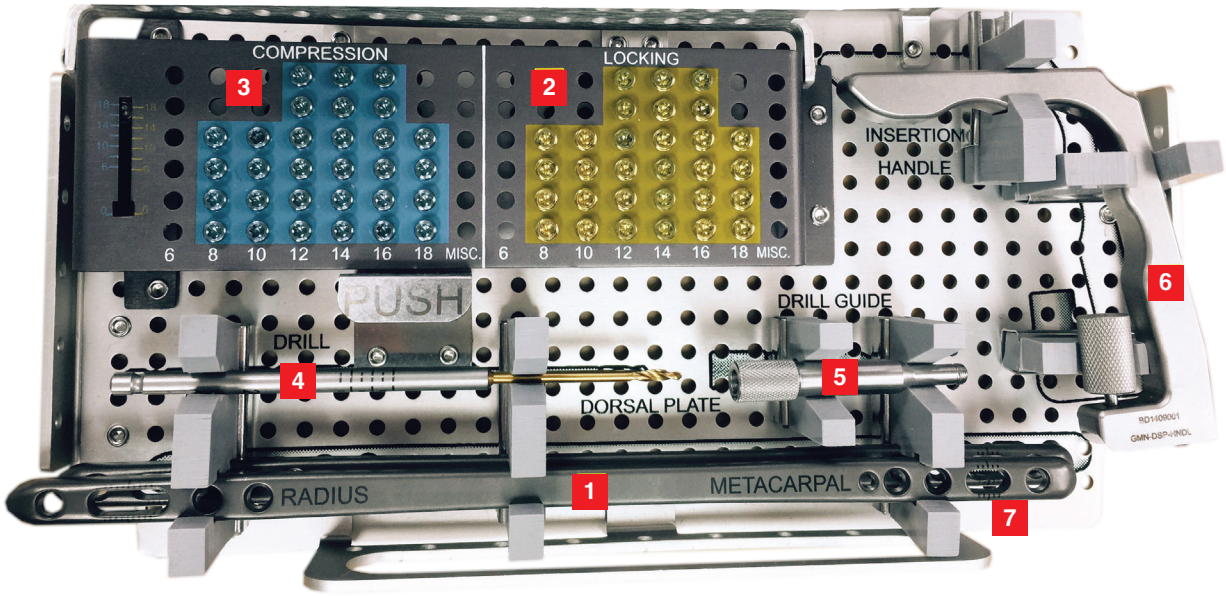

Loc #	Catalog #	Description
1	GMN-DSP-210	Dorsal Spanning Plate (long)
	GMN-DSP-160	Dorsal Spanning Plate (short)
2	MTLS-30080-TS	Screw, Multi-Thread, Locking, 3.0mm x 8mm, Ti
	MTLS-30100-TS	Screw, Multi-Thread, Locking, 3.0mm x 10mm, Ti
	MTLS-30120-TS	Screw, Multi-Thread, Locking, 3.0mm x 12mm, Ti
	MTLS-30140-TS	Screw, Multi-Thread, Locking, 3.0mm x 14mm, Ti
	MTLS-30160-TS	Screw, Multi-Thread, Locking, 3.0mm x 16mm, Ti
	MTLS-30180-TS	Screw, Multi-Thread, Locking, 3.0mm x 18mm, Ti
3	MTNL-30080-TS	Screw, Multi-Thread, Compression, 3.0mm x 8mm, Ti
	MTNL-30100-TS	Screw, Multi-Thread, Compression, 3.0mm x 10mm, Ti
	MTNL-30120-TS	Screw, Multi-Thread, Compression, 3.0mm x 12mm, Ti
	MTNL-30140-TS	Screw, Multi-Thread, Compression, 3.0mm x 14mm, Ti
	MTNL-30160-TS	Screw, Multi-Thread, Compression, 3.0mm x 16mm, Ti
	MTNL-30180-TS	Screw, Multi-Thread, Compression, 3.0mm x 18mm, Ti

INSTRUMENTS

Loc #	Catalog #	Description
4	DRLL-SSC-23040	Drill, 2.3mm X 40mm
5	TPDG-THD-DG23	Thread-In Drill Guide, 2.3mm
6	GMN-DSP-HNDL	Assembled, Handle, Dorsal Spanning Plate
7	GMN-DSP-TRAY	Instrument Tray, Dorsal Spanning Plate


DORSAL SPANNING PLATE



Dorsal Spanning Plate, Long, 210 mm TI



Dorsal Spanning Plate, Short, 160mm TI

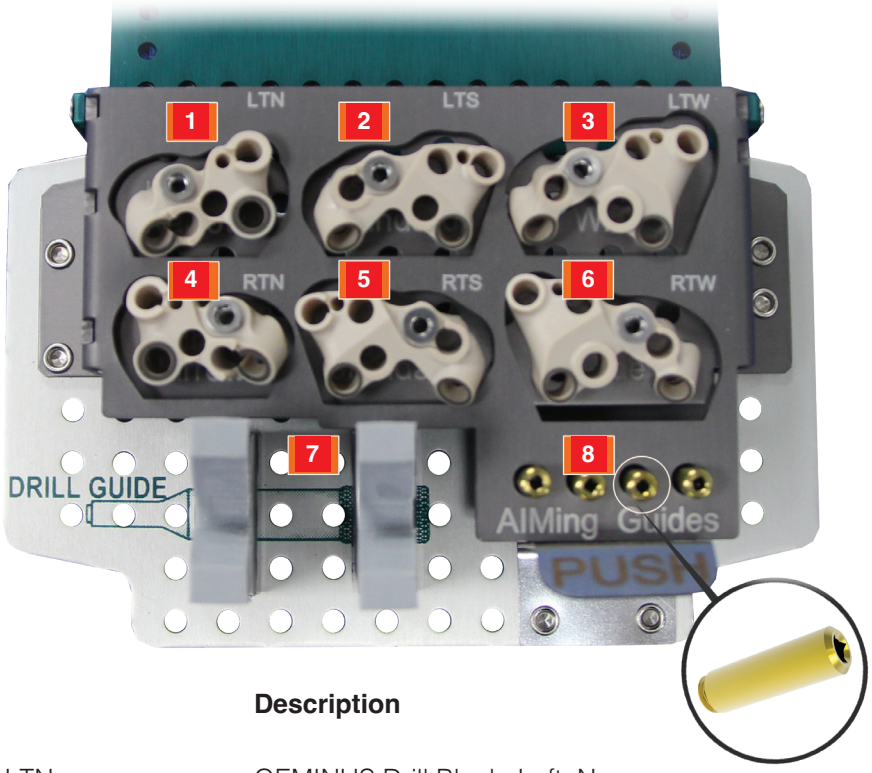

Loc #	Catalog #	Description
1	GMN-DBK-LTN	GEMINUS Drill Block, Left, Narrow
2	GMN-DBK-LTS	GEMINUS Drill Block, Left, Standard
3	GMN-DBK-LTW	GEMINUS Drill Block, Left, Wide
4	GMN-DBK-RTN	GEMINUS Drill Block, Right, Narrow
5	GMN-DBK-RTS	GEMINUS Drill Block, Right, Standard
6	GMN-DBK-RTW	GEMINUS Drill Block, Right, Wide
7	TPDG-THD-DG20	Thread-In Drill Guide, 2.0mm (Located in upper tray)
8	DBK-AIM-015	GEMINUS Drill Block, A.I.M.ing Guide, 1.6mm

Only available in the EU

Catalog #	Description
GMN-RTN-3HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Narrow, 3 Hole, Right Single-pack
GMN-LTN-3HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Narrow, 3 Hole, Left Single-pack
GMN-RTN-4HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Narrow, 4 Hole, Right Single-pack
GMN-LTN-4HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Narrow, 4 Hole, Left Single-pack
GMN-RTS-3HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Standard, 3 Hole, Right Single-pack
GMN-LTS-3HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Standard, 3 Hole, Left Single-pack
GMN-RTS-4HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Standard, 4 Hole, Right Single-pack
GMN-LTS-4HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Standard, 4 Hole, Left Single-pack
GMN-RTS-7HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Standard, 7 Hole, Right Single-pack
GMN-LTS-7HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Standard, 7 Hole, Left Single-pack
GMN-RTW-4HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Wide, 4 Hole, Right Single-pack
GMN-LTW-4HL-S01	Sterile Assembled GEMINUS Volar Distal Radius Plate, Wide, 4 Hole, Left Single-pack
PRT-FSP-LR-S01	Sterile PROTEAN Fragment Plate, Double Hockey Stick Single-pack
PRT-FSP-YS-S01	Sterile PROTEAN Fragment Plate, Y Single-pack
PRT-FSP-DU-S01	Sterile PROTEAN Fragment Plate, Distal Ulna Single-pack
PRT-FSP-SR2-S01	Sterile PROTEAN Fragment Plate, Scapholunate, Long, Right Single-pack
PRT-FSP-SL2-S01	Sterile PROTEAN Fragment Plate, Scapholunate, Long, Left Single-pack
PRT-FSP-SR1-S01	Sterile PROTEAN Fragment Plate, Scapholunate, Short, Right Single-pack
PRT-FSP-SL1-S01	Sterile PROTEAN Fragment Plate, Scapholunate, Short, Left Single-pack
PRT-RCP-RT-S01	Sterile PROTEAN Fragment Plate, Radial Column Plate, Right Single-pack
PRT-RCP-LT-S01	Sterile PROTEAN Fragment Plate, Radial Column Plate, Left Single-pack
PRT-CCP-RT-S01	Sterile PROTEAN Fragment Plate, Central Column Plate, Right Single-pack
PRT-CCP-LT-S01	Sterile PROTEAN Fragment Plate, Central Column Plate, Left Single-pack
SPLS-20140-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 14mm, Ti Single-pack
SPLS-20160-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 16mm, Ti Single-pack
SPLS-20170-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 17mm, Ti Single-pack
SPLS-20180-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 18mm, Ti Single-pack
SPLS-20190-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 19mm, Ti Single-pack
SPLS-20200-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 20mm, Ti Single-pack
SPLS-20210-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 21mm, Ti Single-pack
SPLS-20220-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 22mm, Ti Single-pack
SPLS-20230-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 23mm, Ti Single-pack
SPLS-20240-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 24mm, Ti Single-pack
SPLS-20260-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 26mm, Ti Single-pack
SPLS-20280-TS-S01	Sterile Smooth Peg, Locking, 2.0mm x 28mm, Ti Single-pack
TPLS-23100-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 10mm, Ti Single-pack
TPLS-23120-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 12mm, Ti Single-pack
TPLS-23140-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 14mm, Ti Single-pack
TPLS-23160-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 16mm, Ti Single-pack
TPLS-23170-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 17mm, Ti Single-pack
TPLS-23180-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 18mm, Ti Single-pack
TPLS-23190-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 19mm, Ti Single-pack
TPLS-23200-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 20mm, Ti Single-pack
TPLS-23210-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 21mm, Ti Single-pack
TPLS-23220-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 22mm, Ti Single-pack
TPLS-23230-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 23mm, Ti Single-pack
TPLS-23240-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 24mm, Ti Single-pack
TPLS-23260-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 26mm, Ti Single-pack
TPLS-23280-TS-S01	Sterile Threaded Peg, Locking, 2.3mm x 28mm, Ti Single-pack

EU STERILE PRODUCT LIST

Only available in the EU

Catalog #	Description
HCLP-27100-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 10mm, Ti Single-pack
HCLP-27120-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 12mm, Ti Single-pack
HCLP-27140-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 14mm, Ti Single-pack
HCLP-27160-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 16mm, Ti Single-pack
HCLP-27180-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 18mm, Ti Single-pack
HCLP-27190-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 19mm, Ti Single-pack
HCLP-27200-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 20mm, Ti Single-pack
HCLP-27210-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 21mm, Ti Single-pack
HCLP-27220-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 22mm, Ti Single-pack
HCLP-27230-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 23mm, Ti Single-pack
HCLP-27240-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 24mm, Ti Single-pack
HCLP-27260-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 26mm, Ti Single-pack
HCLP-27280-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 28mm, Ti Single-pack
HCLP-27300-TS-S01	Sterile High Compression Locking Peg, 2.7mm x 30mm, Ti Single-pack
TPNL-27100-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 10mm, Ti Single-pack
TPNL-27120-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 12mm, Ti Single-pack
TPNL-27140-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 14mm, Ti Single-pack
TPNL-27160-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 16mm, Ti Single-pack
TPNL-27180-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 18mm, Ti Single-pack
TPNL-27200-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 20mm, Ti Single-pack
TPNL-27220-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 22mm, Ti Single-pack
TPNL-27240-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 24mm, Ti Single-pack
TPNL-27260-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 26mm, Ti Single-pack
TPNL-27280-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 28mm, Ti Single-pack
TPNL-27300-TS-S01	Sterile Threaded Peg, Non-Locking, 2.7mm x 30mm, Ti Single-pack
WBTN-2750-T-S01	Sterile Washer, Button Single-pack
PANL-35080-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 8mm, Ti Single-pack
PANL-35090-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 9mm, Ti Single-pack
PANL-35100-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 10mm, Ti Single-pack
PANL-35110-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 11mm, Ti Single-pack
PANL-35120-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 12mm, Ti Single-pack
PANL-35130-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 13mm, Ti Single-pack
PANL-35140-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 14mm, Ti Single-pack
PANL-35150-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 15mm, Ti Single-pack
PANL-35160-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 16mm, Ti Single-pack
PANL-35180-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 18mm, Ti Single-pack
COLS-35080-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 8mm, Ti Single-pack
COLS-35090-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 9mm, Ti Single-pack
COLS-35100-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 10mm, Ti Single-pack
COLS-35110-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 11mm, Ti Single-pack
COLS-35120-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 12mm, Ti Single-pack
COLS-35130-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 13mm, Ti Single-pack
COLS-35140-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 14mm, Ti Single-pack
COLS-35150-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 15mm, Ti Single-pack
COLS-35160-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 16mm, Ti Single-pack
COLS-35180-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 18mm, Ti Single-pack
PALS-25100-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 10mm Cannulated, CoCr Single-pack
PALS-25120-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 12mm Cannulated, CoCr Single-pack

EU STERILE PRODUCT LIST

Only available in the EU

Catalog #	Description
PALS-25140-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 14mm Cannulated, CoCr Single-pack
PALS-25160-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 16mm Cannulated, CoCr Single-pack
PALS-25180-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 18mm Cannulated, CoCr Single-pack
PALS-25200-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 20mm Cannulated, CoCr Single-pack
PALS-25220-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 22mm Cannulated, CoCr Single-pack
PALS-25240-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 24mm Cannulated, CoCr Single-pack
PALS-25260-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 26mm Cannulated, CoCr Single-pack
PALS-25280-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 28mm Cannulated, CoCr Single-pack
GMN-HP-S01	Sterile GEMINUS Hook Plate Single-pack
GMN-HP-SCRW-S01	Sterile GEMINUS Hook Plate, Screw Single-pack
GMN-RTN-120-S01	Sterile Assembled, GEMINUS VDR Plate, Narrow, 120mm, Right Single-pack
GMN-LTN-120-S01	Sterile Assembled, GEMINUS VDR Plate, Narrow, 120mm, Left Single-pack
GMN-RTN-160-S01	Sterile Assembled, GEMINUS VDR Plate, Narrow, 160mm, Right Single-pack
GMN-LTN-160-S01	Sterile Assembled, GEMINUS VDR Plate, Narrow, 160mm, Left Single-pack
GMN-RTN-200-S01	Sterile Assembled, GEMINUS VDR Plate, Narrow, 200mm, Right Single-pack
GMN-LTN-200-S01	Sterile Assembled, GEMINUS VDR Plate, Narrow, 200mm, Left Single-pack
GMN-RTS-120-S01	Sterile Assembled, GEMINUS VDR Plate, Standard, 120mm, Right Single-pack
GMN-LTS-120-S01	Sterile Assembled, GEMINUS VDR Plate, Standard, 120mm, Left Single-pack
GMN-RTS-160-S01	Sterile Assembled, GEMINUS VDR Plate, Standard, 160mm, Right Single-pack
GMN-LTS-160-S01	Sterile Assembled, GEMINUS VDR Plate, Standard, 160mm, Left Single-pack
GMN-RTS-200-S01	Sterile Assembled, GEMINUS VDR Plate, Standard, 200mm, Right Single-pack
GMN-LTS-200-S01	Sterile Assembled, GEMINUS VDR Plate, Standard, 200mm, Left Single-pack
PANL-35080-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 8mm, Ti Single-pack
PANL-35090-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 9mm, Ti Single-pack
PANL-35100-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 10mm, Ti Single-pack
PANL-35110-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 11mm, Ti Single-pack
PANL-35120-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 12mm, Ti Single-pack
PANL-35130-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 13mm, Ti Single-pack
PANL-35140-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 14mm, Ti Single-pack
PANL-35150-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 15mm, Ti Single-pack
PANL-35160-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 16mm, Ti Single-pack
PANL-35180-TS-S01	Sterile Screw, Cortical Non Locking, 3.5mm x 18mm, Ti Single-pack
COLS-35080-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 8mm, Ti Single-pack
COLS-35090-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 9mm, Ti Single-pack
COLS-35100-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 10mm, Ti Single-pack
COLS-35110-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 11mm, Ti Single-pack
COLS-35120-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 12mm, Ti Single-pack
COLS-35130-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 13mm, Ti Single-pack
COLS-35140-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 14mm, Ti Single-pack
COLS-35150-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 15mm, Ti Single-pack
COLS-35160-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 16mm, Ti Single-pack
COLS-35180-TS-S01	Sterile Screw, Cortical Locking, 3.5mm x 18mm, Ti Single-pack
PALS-25100-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 10mm Cannulated, CoCr Single-pack
PALS-25120-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 12mm Cannulated, CoCr Single-pack
PALS-25140-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 14mm Cannulated, CoCr Single-pack
PALS-25160-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 16mm Cannulated, CoCr Single-pack
PALS-25180-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 18mm Cannulated, CoCr Single-pack
PALS-25200-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 20mm Cannulated, CoCr Single-pack

EU STERILE PRODUCT LIST

Only available in the EU

Catalog #	Description
PALS-25220-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 22mm Cannulated, CoCr Single-pack
PALS-25240-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 24mm Cannulated, CoCr Single-pack
PALS-25260-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 26mm Cannulated, CoCr Single-pack
PALS-25280-CC-S01	Sterile Screw, Polyaxial Locking, 2.5mm x 28mm Cannulated, CoCr Single-pack
GMN-HP-S01	Sterile GEMINUS Hook Plate Single-pack
GMN-HP-RR-S01	Sterile GEMINUS Hook Plate, Radial, Right Single-pack
GMN-HP-RL-S01	Sterile GEMINUS Hook Plate, Radial, Left Single-pack
GMN-HP-SCRW-S01	Sterile GEMINUS Hook Plate, Screw Single-pack
BB-RND-01-S01	Sterile Buttress Button, 6.35mm Round, 0.6mm x 152mm Single-pack

skeletal dynamics®

CE 2797
MKT-00005-00 V.3
May 2026

© 2026 Skeletal Dynamics
7300 North Kendall Drive, Suite 800, Miami, Florida 33156, 877-753-5396
Designed and Manufactured in the USA

EC REP
EMERGO EUROPE
Westervoortsedijk 60
6827 AT Arnhem
The Netherlands